

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV080618\
 Data File : VV006896.D
 Acq On : 06 Aug 2018 12:34
 Operator : SY/MD
 Sample : VV0806WBL01
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK80

Quant Time: Aug 07 09:40:48 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080218WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Aug 06 03:23:10 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	258831	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	248994	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	97075	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	91150	5.08	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	101.60%
7) Chloroethane-d5	1.58	69	87195	5.59	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	111.80%
11) 1,1-Dichloroethene-d2	2.13	63	137254	4.13	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	82.60%
20) 2-Butanone-d5	3.96	46	224242	51.58	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	103.16%
24) Chloroform-d	4.40	84	177838	5.67	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	113.40%
26) 1,2-Dichloroethane-d4	5.09	65	93735	5.92	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	118.40%
32) Benzene-d6	5.10	84	332739	4.95	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.00%
36) 1,2-Dichloropropane-d6	6.12	67	116151	5.23	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	104.60%
41) Toluene-d8	7.36	98	251441	4.19	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.80%
43) trans-1,3-Dichloropropene-	7.67	79	35705	4.55	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.00%
46) 2-Hexanone-d5	8.14	63	133449	38.18	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	76.36%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	86273	5.22	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	104.40%
64) 1,2-Dichlorobenzene-d4	11.68	152	88980	4.94	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.80%


Target Compounds					Ovalue
16) Methylene chloride	2.54	84	13227	0.67 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV080618\
Data File : VV006896.D
Acq On : 06 Aug 2018 12:34
Operator : SY/MD
Sample : VV0806WBL01
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK80

Quant Time: Aug 07 09:40:48 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080218WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Aug 06 03:23:10 2018
Response via : Initial Calibration

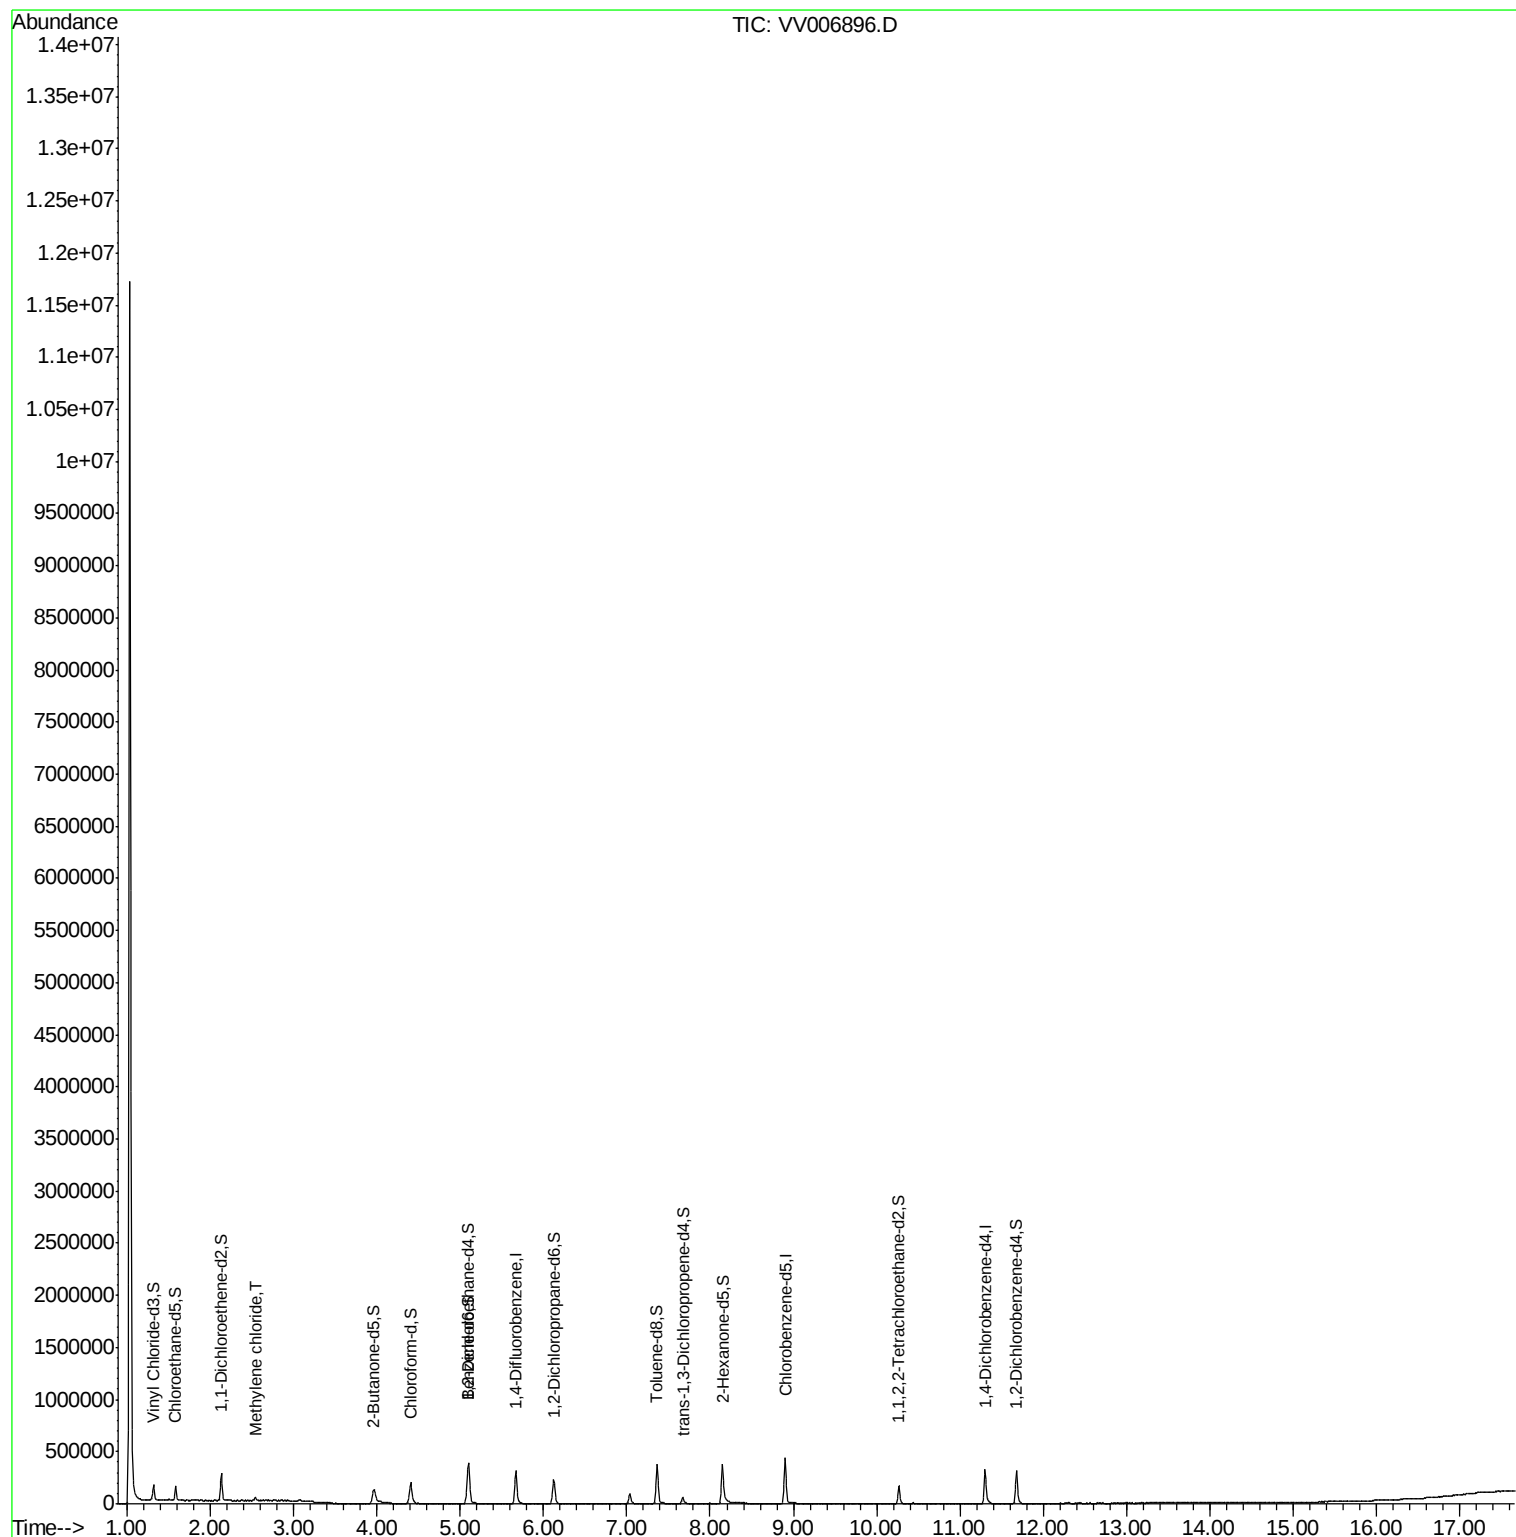

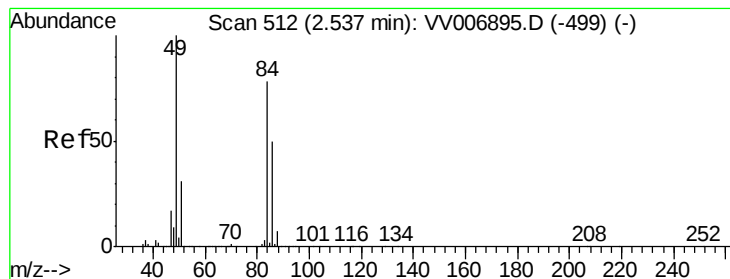

#16

Methylene chloride

Concen: 0.67 ug/L

RT: 2.54 min Scan# 512

Delta R.T. -0.00 min

Lab File: VV006896.D

Acq: 06 Aug 2018 12:34

Instrument :

MSVOA_V

ClientSampleId :

VBLK80


Tot Ion: 84 Resp: 13227

Ion Ratio Lower Upper

84 100

86 62.2 43.8 81.3

49 123.0 85.3 158.5

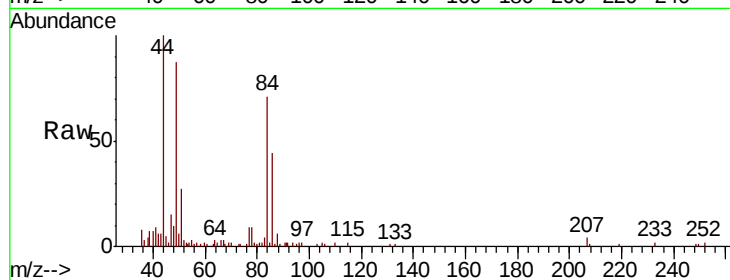

Abundance Ion 84.05 (83.75 to 84.75): VV0

Ion 86.00 (85.70 to 86.70): VV0

Ion 49.10 (48.80 to 49.80): VV0

