


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV080619\
Data File : VV012105.D
Acq On : 06 Aug 2019 09:19
Operator : SY/MD
Sample : BFB45
Misc : 25mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB611

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM080619W.M
Title : VOC Analysis
Last Update : Wed Aug 07 18:21:59 2019

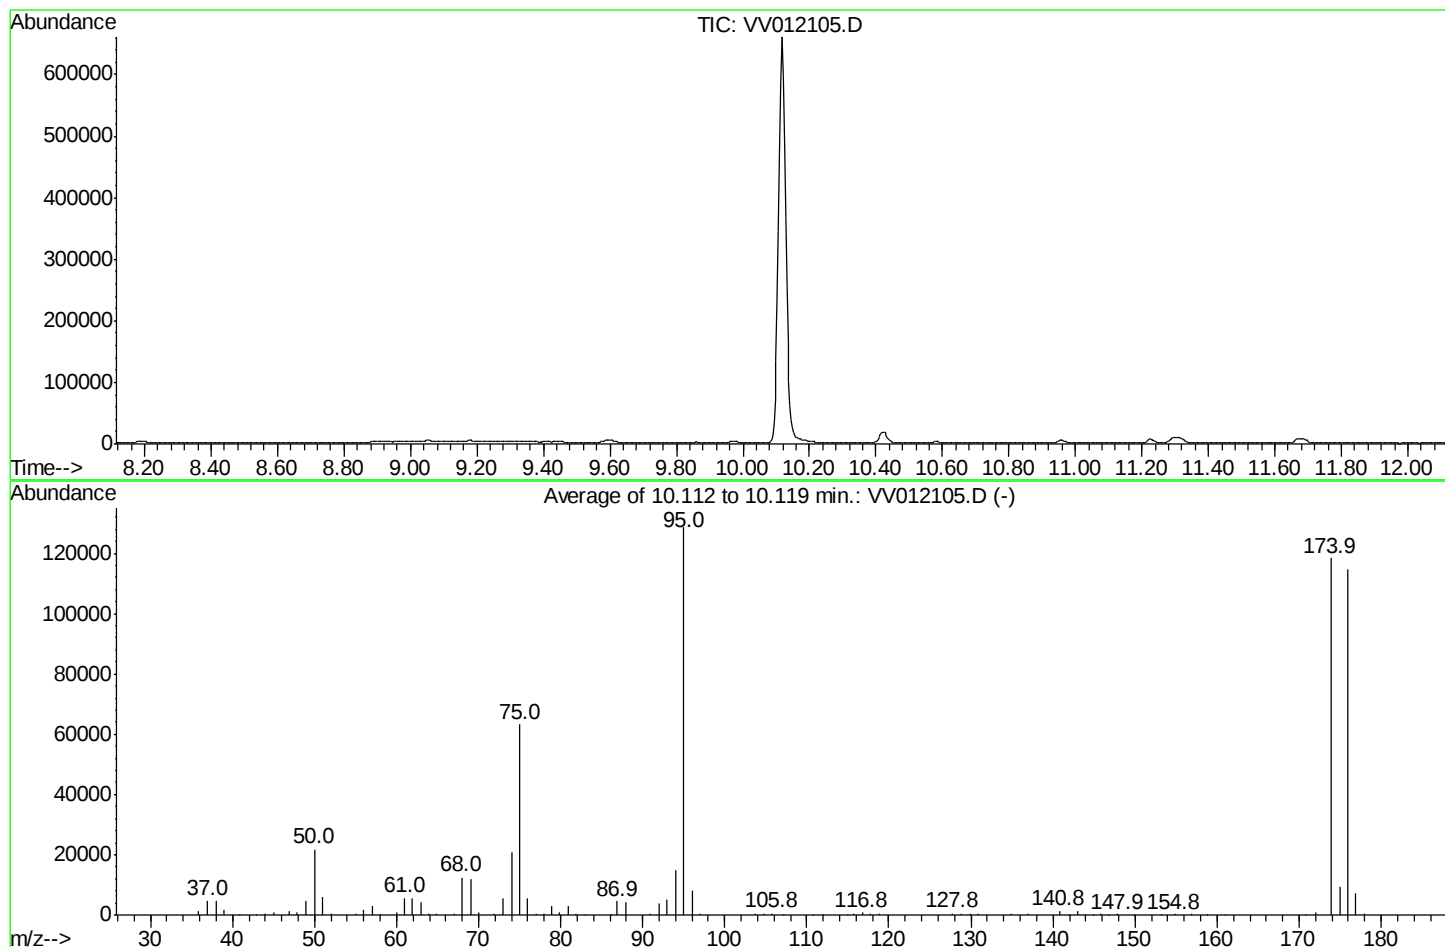

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	21701	PASS
75	95	30	80	49.1	63157	PASS
95	95	100	100	100.0	128664	PASS
96	95	5	9	6.3	8053	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	92.1	118490	PASS
175	174	5	9	7.8	9295	PASS
176	174	95	101	97.0	114917	PASS
177	176	5	9	6.4	7411	PASS

Scan 2794 (10.074 min): VV012105.D
BFB45

m/z	Abundance
35.90	978.0
38.10	309.0
39.80	396.0
43.90	251.0

Instrument :
MSVOA_V
ClientSampleId :
BFB611

m/z	Abundance
36.00	2087.0
37.00	4938.0
38.00	5078.0
39.00	1941.0
39.90	275.0
43.90	749.0
45.00	898.0
46.90	1361.0
47.90	742.0
49.00	4770.0
50.00	22496.0
51.00	6191.0
52.00	400.0
55.00	319.0
56.00	2007.0
57.00	2886.0
58.10	110.0
60.00	1103.0
61.00	5812.0
61.90	5697.0
63.00	4511.0
63.90	504.0
64.90	415.0
67.00	427.0
68.00	13068.0
69.00	12584.0
69.90	863.0
71.90	617.0
72.90	5865.0
74.00	21456.0
75.00	65360.0
76.00	5641.0
77.00	559.0
78.00	480.0
78.90	3160.0
79.80	953.0
80.90	2948.0
81.90	593.0
86.00	189.0
86.90	4847.0
87.90	4494.0
90.90	488.0
91.90	4019.0
92.90	5383.0
94.00	15217.0
95.00	133184.0
96.00	8294.0
97.00	391.0
103.80	412.0
104.80	252.0
105.80	568.0
107.10	115.0
110.70	101.0
111.90	117.0
114.90	136.0
115.80	562.0
116.80	697.0
117.80	478.0
118.80	616.0
127.80	558.0
128.80	275.0
129.80	522.0
130.80	256.0
134.80	257.0
137.00	265.0
140.80	1491.0
141.80	168.0
143.00	1347.0
144.00	108.0
144.90	168.0
145.80	249.0
147.90	326.0
149.90	191.0
154.90	335.0
156.90	287.0
158.80	147.0
160.90	214.0
170.80	165.0
172.00	705.0
173.90	122304.0
174.90	9607.0
175.90	118632.0
176.90	7691.0
178.00	270.0

Instrument :
MSVOA_V
ClientSampleId :
BFB611

m/z	Abundance
36.00	1997.0
37.00	4502.0
38.00	4638.0
39.00	1759.0
39.90	306.0
42.90	117.0
43.90	695.0
45.00	866.0
46.90	1162.0
47.90	675.0
49.00	4261.0
50.00	20264.0
51.00	5825.0
52.00	418.0
54.90	281.0
55.90	1745.0
57.00	2535.0
58.10	111.0
60.00	1018.0
61.00	5308.0
61.90	5198.0
63.00	4165.0
63.90	532.0
64.90	412.0
67.00	407.0
68.00	11666.0
69.00	11525.0
70.00	864.0
71.90	623.0
72.90	5254.0
74.00	19280.0
75.00	59632.0
76.00	5184.0
77.00	511.0
77.90	442.0
78.90	2973.0
79.80	829.0
80.90	2669.0
81.90	529.0
83.00	109.0
86.10	145.0
86.90	4306.0
87.90	3940.0
90.90	448.0
92.00	3537.0
92.90	4866.0
94.00	13481.0
95.00	120584.0
96.00	7464.0
97.00	319.0
103.70	359.0
104.80	267.0
105.80	564.0
107.10	105.0
115.00	114.0
115.80	511.0
116.70	563.0
117.80	441.0
118.80	655.0
127.80	479.0
128.80	202.0
129.90	495.0
130.80	231.0
134.90	248.0
137.00	194.0
140.80	1257.0
141.80	151.0
142.90	1189.0
144.80	158.0
145.80	246.0
146.80	112.0
147.90	263.0
150.00	190.0
154.90	325.0
156.90	269.0
160.90	184.0
170.80	117.0
172.10	650.0
173.90	107360.0
174.90	8448.0
175.90	104184.0
176.90	6905.0
177.90	226.0

Instrument :
MSVOA_V
ClientSampleId :
BFB611

m/z	Abundance
36.00	1997.0
37.00	4502.0
38.00	4638.0
39.00	1759.0
39.90	306.0
42.90	117.0
43.90	695.0
45.00	866.0
46.90	1162.0
47.90	675.0
49.00	4261.0
50.00	20264.0
51.00	5825.0
52.00	418.0
54.90	281.0
55.90	1745.0
57.00	2535.0
58.10	111.0
60.00	1018.0
61.00	5308.0
61.90	5198.0
63.00	4165.0
63.90	532.0
64.90	412.0
67.00	407.0
68.00	11666.0
69.00	11525.0
70.00	864.0
71.90	623.0
72.90	5254.0
74.00	19280.0
75.00	59632.0
76.00	5184.0
77.00	511.0
77.90	442.0
78.90	2973.0
79.80	829.0
80.90	2669.0
81.90	529.0
83.00	109.0
86.10	145.0
86.90	4306.0
87.90	3940.0
90.90	448.0
92.00	3537.0
92.90	4866.0
94.00	13481.0
95.00	120584.0
96.00	7464.0
97.00	319.0
103.70	359.0
104.80	267.0
105.80	564.0
107.10	105.0
115.00	114.0
115.80	511.0
116.70	563.0
117.80	441.0
118.80	655.0
127.80	479.0
128.80	202.0
129.90	495.0
130.80	231.0
134.90	248.0
137.00	194.0
140.80	1257.0
141.80	151.0
142.90	1189.0
144.80	158.0
145.80	246.0
146.80	112.0
147.90	263.0
150.00	190.0
154.90	325.0
156.90	269.0
160.90	184.0
170.80	117.0
172.10	650.0
173.90	107360.0
174.90	8448.0
175.90	104184.0
176.90	6905.0
177.90	226.0

Instrument :
MSVOA_V
ClientSampleId :
BFB611

m/z	Abundance
35.90	2100.0
37.00	4963.0
38.00	5161.0
39.00	1913.0
40.00	269.0
40.90	101.0
43.90	758.0
45.00	827.0
46.90	1320.0
47.90	729.0
49.00	4648.0
50.00	22344.0
51.00	6257.0
52.00	323.0
55.00	305.0
56.00	1938.0
57.00	3001.0
58.00	116.0
59.90	1076.0
61.00	5799.0
61.90	5496.0
63.00	4439.0
63.90	449.0
64.90	345.0
67.00	394.0
67.90	12728.0
69.00	12260.0
70.00	779.0
71.90	589.0
72.90	5791.0
74.00	21352.0
75.00	64480.0
76.00	5582.0
76.90	620.0
78.00	483.0
78.90	3046.0
79.80	974.0
80.90	2916.0
81.90	679.0
86.00	200.0
86.90	4737.0
87.90	4519.0
90.90	468.0
91.90	3817.0
93.00	5561.0
94.00	15454.0
95.00	132224.0
96.00	8401.0
97.00	398.0
103.80	456.0
104.80	207.0
105.80	526.0
110.70	102.0
111.90	142.0
114.80	155.0
115.70	522.0
116.80	799.0
117.80	513.0
118.80	573.0
127.80	594.0
128.90	318.0
129.80	516.0
130.80	227.0
134.80	268.0
136.90	301.0
140.80	1528.0
141.90	195.0
142.90	1459.0
144.00	104.0
144.80	158.0
145.70	253.0
147.90	392.0
149.80	166.0
153.10	110.0
154.80	327.0
156.90	277.0
158.80	201.0
160.90	179.0
170.70	186.0
172.00	646.0
173.90	125808.0
175.00	9832.0
175.90	121936.0
176.90	7637.0
178.00	287.0

Instrument :
MSVOA_V
ClientSampleId :
BFB611