
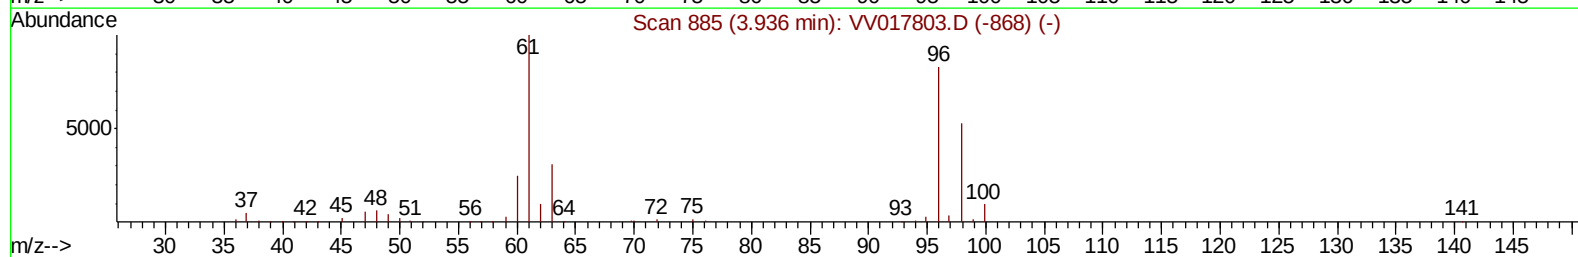
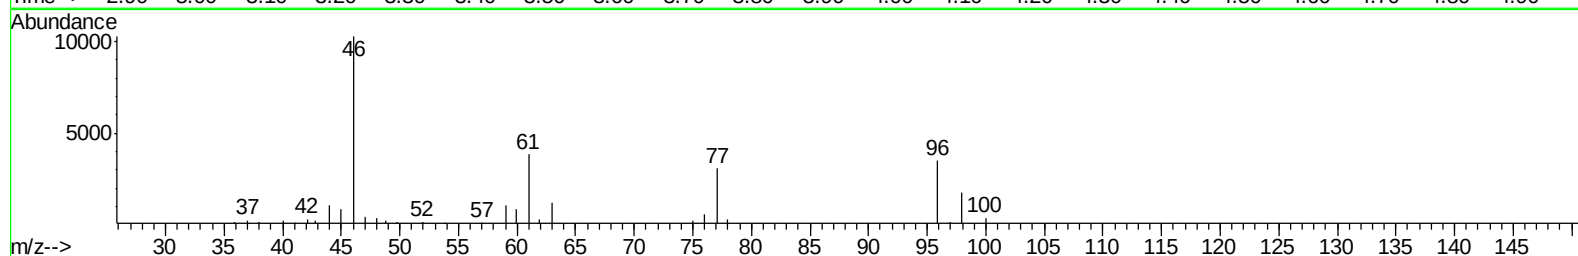


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV080620\  
Data File : VV017814.D  
Acq On : 06 Aug 2020 15:13  
Operator : SY/MD  
Sample : L3590-08  
Misc : 5.0mL/MSVOA V/WATER  
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Aug 07 05:30:59 2020  
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_V\METHOD\SOMVLM073020WMA.M  
Quant Title : VOC Analysis  
QLast Update : Fri Aug 07 05:27:52 2020  
Response via : Initial Calibration

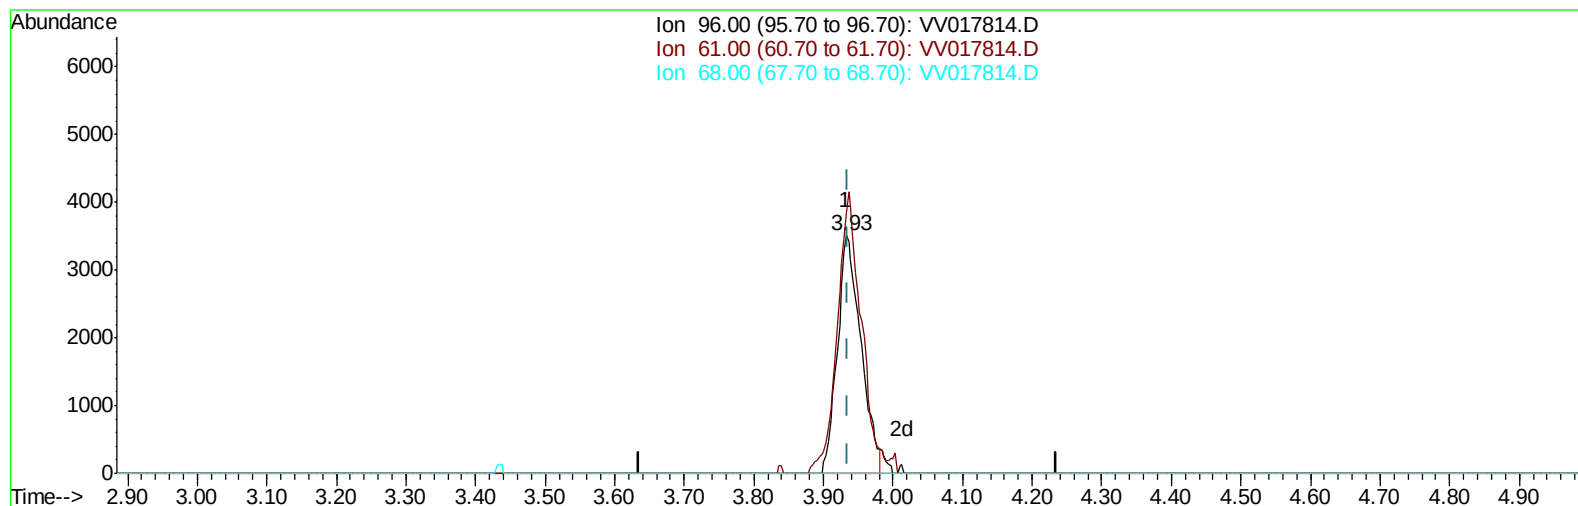

TIC: VV017814.D

(20) cis-1,2-Dichloroethene (T)

3.933min (-0.003) 6.14ug/L

response 8220

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 96.00 | 100    | 100    |
| 61.00 | 124.70 | 109.75 |
| 68.00 | 0.00   | 0.00   |
| 0.00  | 0.00   | 0.00   |