

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV080620\
 Data File : VV017814.D
 Acq On : 06 Aug 2020 15:13
 Operator : SY/MD
 Sample : L3590-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F2L53

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM073020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.775	514	524	537	rBV2	11729	20697	3.17%	0.437%
2	3.010	595	597	598	rBV2	356	118	0.02%	0.002%
3	3.061	608	613	615	rBV	419	386	0.06%	0.008%
4	3.103	624	626	628	rBV2	412	144	0.02%	0.003%
5	3.154	639	642	643	rBV2	268	157	0.02%	0.003%
6	3.216	658	661	663	rBV2	602	334	0.05%	0.007%
7	3.241	668	669	671	rBB2	111	41	0.01%	0.001%
8	3.254	671	673	674	rBB2	121	46	0.01%	0.001%
9	3.270	674	678	679	rBV	292	201	0.03%	0.004%
10	3.344	693	701	702	rBV	543	504	0.08%	0.011%
11	3.402	715	719	720	rBV	433	272	0.04%	0.006%
12	3.450	733	734	736	rBB	107	41	0.01%	0.001%
13	3.463	736	738	739	rBV	344	133	0.02%	0.003%
14	3.489	743	746	748	rVV	416	261	0.04%	0.006%
15	3.505	748	751	754	rVB	206	137	0.02%	0.003%
16	3.576	771	773	775	rBV2	276	177	0.03%	0.004%
17	3.656	795	798	802	rBV2	420	382	0.06%	0.008%
18	3.740	822	824	825	rBV2	234	92	0.01%	0.002%
19	3.756	827	829	831	rBB	121	68	0.01%	0.001%
20	3.769	831	833	834	rBB	118	42	0.01%	0.001%
21	3.794	839	841	844	rVV	267	116	0.02%	0.002%
22	3.855	858	860	862	rBV2	328	105	0.02%	0.002%
23	3.907	865	876	905	rBV4	44893	160392	24.55%	3.385%
24	4.315	998	1003	1005	rBV2	406	290	0.04%	0.006%
25	4.373	1005	1021	1042	rBV	120283	295952	45.31%	6.247%
26	4.675	1113	1115	1120	rBB2	578	375	0.06%	0.008%
27	4.698	1120	1122	1124	rBB	243	111	0.02%	0.002%
28	4.746	1134	1137	1138	rBV	257	144	0.02%	0.003%
29	4.810	1156	1157	1158	rBB	105	20	0.00%	0.000%
30	4.833	1159	1164	1165	rBV	463	303	0.05%	0.006%
31	4.881	1178	1179	1180	rBV	245	76	0.01%	0.002%
32	4.968	1205	1206	1210	rBV	142	53	0.01%	0.001%
33	4.987	1210	1212	1216	rVB	358	263	0.04%	0.006%
34	5.010	1217	1219	1220	rBV	388	184	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV080620\
 Data File : VV017814.D
 Acq On : 06 Aug 2020 15:13
 Operator : SY/MD
 Sample : L3590-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F2L53

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM073020WMA.M
 Title : VOC Analysis

35	5.071	1221	1238	1259	rBV2	251610	653241	100.00%	13.788%
36	5.228	1285	1287	1289	rBV	209	113	0.02%	0.002%
37	5.289	1302	1306	1309	rBV3	580	522	0.08%	0.011%
38	5.389	1332	1337	1339	rBV3	494	331	0.05%	0.007%
39	5.402	1339	1341	1344	rBV2	393	270	0.04%	0.006%
40	5.453	1352	1357	1363	rBV2	405	517	0.08%	0.011%
41	5.521	1375	1378	1379	rBB	233	108	0.02%	0.002%
42	5.537	1382	1383	1386	rBV	317	190	0.03%	0.004%
43	5.569	1390	1393	1397	rBB	351	303	0.05%	0.006%
44	5.640	1402	1415	1437	rBV	220114	445841	68.25%	9.411%
45	6.823	1781	1783	1785	rBV	462	207	0.03%	0.004%
46	6.891	1802	1804	1806	rBV	271	164	0.03%	0.003%
47	6.907	1806	1809	1811	rVV2	701	414	0.06%	0.009%
48	7.010	1831	1841	1857	rBV2	39158	69877	10.70%	1.475%
49	7.270	1919	1922	1924	rVB	383	208	0.03%	0.004%
50	7.338	1930	1943	1961	rBV	316175	546527	83.66%	11.536%
51	7.531	2000	2003	2009	rBB3	611	616	0.09%	0.013%
52	7.559	2009	2012	2018	rBB3	647	600	0.09%	0.013%
53	7.592	2018	2022	2025	rBB3	697	510	0.08%	0.011%
54	7.643	2029	2038	2061	rVB2	46475	79114	12.11%	1.670%
55	7.788	2081	2083	2087	rVB	397	233	0.04%	0.005%
56	7.813	2087	2091	2095	rVB4	751	658	0.10%	0.014%
57	7.830	2095	2096	2097	rBV4	234	88	0.01%	0.002%
58	7.878	2109	2111	2117	rBB2	503	381	0.06%	0.008%
59	7.910	2118	2121	2122	rBV	418	172	0.03%	0.004%
60	7.920	2122	2124	2125	rBV	228	56	0.01%	0.001%
61	7.945	2130	2132	2135	rBV	417	302	0.05%	0.006%
62	7.994	2143	2147	2148	rBV2	2353	1593	0.24%	0.034%
63	8.032	2157	2159	2160	rBV	475	185	0.03%	0.004%
64	8.106	2172	2182	2207	rBV	158739	297800	45.59%	6.286%
65	8.450	2287	2289	2291	rVB2	554	213	0.03%	0.004%
66	8.588	2330	2332	2336	rBB	222	146	0.02%	0.003%
67	8.611	2336	2339	2341	rBV2	547	295	0.05%	0.006%
68	8.685	2360	2362	2365	rVB2	453	233	0.04%	0.005%
69	8.772	2383	2389	2393	rBV2	782	809	0.12%	0.017%
70	8.875	2409	2421	2439	rBV	340908	559873	85.71%	11.817%
71	9.074	2480	2483	2485	rBV2	180	155	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV080620\
 Data File : VV017814.D
 Acq On : 06 Aug 2020 15:13
 Operator : SY/MD
 Sample : L3590-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F2L53

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM073020WMA.M
 Title : VOC Analysis

72	9.125	2496	2499	2500	rBV	425	234	0.04%	0.005%
73	9.276	2543	2546	2547	rBV	313	195	0.03%	0.004%
74	9.338	2563	2565	2566	rBV	155	49	0.01%	0.001%
75	9.344	2566	2567	2570	rVB	565	198	0.03%	0.004%
76	9.572	2636	2638	2639	rBV	473	172	0.03%	0.004%
77	9.685	2668	2673	2675	rBV	693	390	0.06%	0.008%
78	9.987	2764	2767	2770	rBV	582	526	0.08%	0.011%
79	10.071	2789	2793	2795	rBV	411	227	0.03%	0.005%
80	10.183	2827	2828	2830	rBV	146	53	0.01%	0.001%
81	10.238	2834	2845	2868	rVB2	220709	338276	51.78%	7.140%
82	10.318	2868	2870	2871	rBV2	291	134	0.02%	0.003%
83	10.405	2894	2897	2902	rVB2	480	297	0.05%	0.006%
84	10.469	2915	2917	2919	rBV2	249	145	0.02%	0.003%
85	10.611	2954	2961	2966	rBV3	720	1111	0.17%	0.023%
86	10.665	2977	2978	2980	rVB	280	79	0.01%	0.002%
87	10.845	3031	3034	3037	rBV	248	201	0.03%	0.004%
88	10.958	3062	3069	3079	rBV5	5330	8161	1.25%	0.172%
89	11.071	3101	3104	3107	rBV2	531	416	0.06%	0.009%
90	11.128	3119	3122	3123	rBV2	356	240	0.04%	0.005%
91	11.270	3155	3166	3188	rBV	391946	603370	92.37%	12.736%
92	11.399	3204	3206	3209	rBV	273	157	0.02%	0.003%
93	11.646	3272	3283	3300	rBV	412199	635910	97.35%	13.422%
94	11.833	3340	3341	3342	rBV	287	85	0.01%	0.002%
95	11.874	3351	3354	3356	rBV2	406	301	0.05%	0.006%
96	11.900	3361	3362	3363	rBV2	329	110	0.02%	0.002%
97	13.077	3724	3728	3730	rBV	438	338	0.05%	0.007%
98	13.228	3774	3775	3778	rBV	580	315	0.05%	0.007%
99	14.736	4241	4244	4247	rBV	675	516	0.08%	0.011%


Sum of corrected areas: 4737688

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV080620\
Data File : VV017814.D
Acq On : 06 Aug 2020 15:13
Operator : SY/MD
Sample : L3590-08
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F2L53

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM073020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

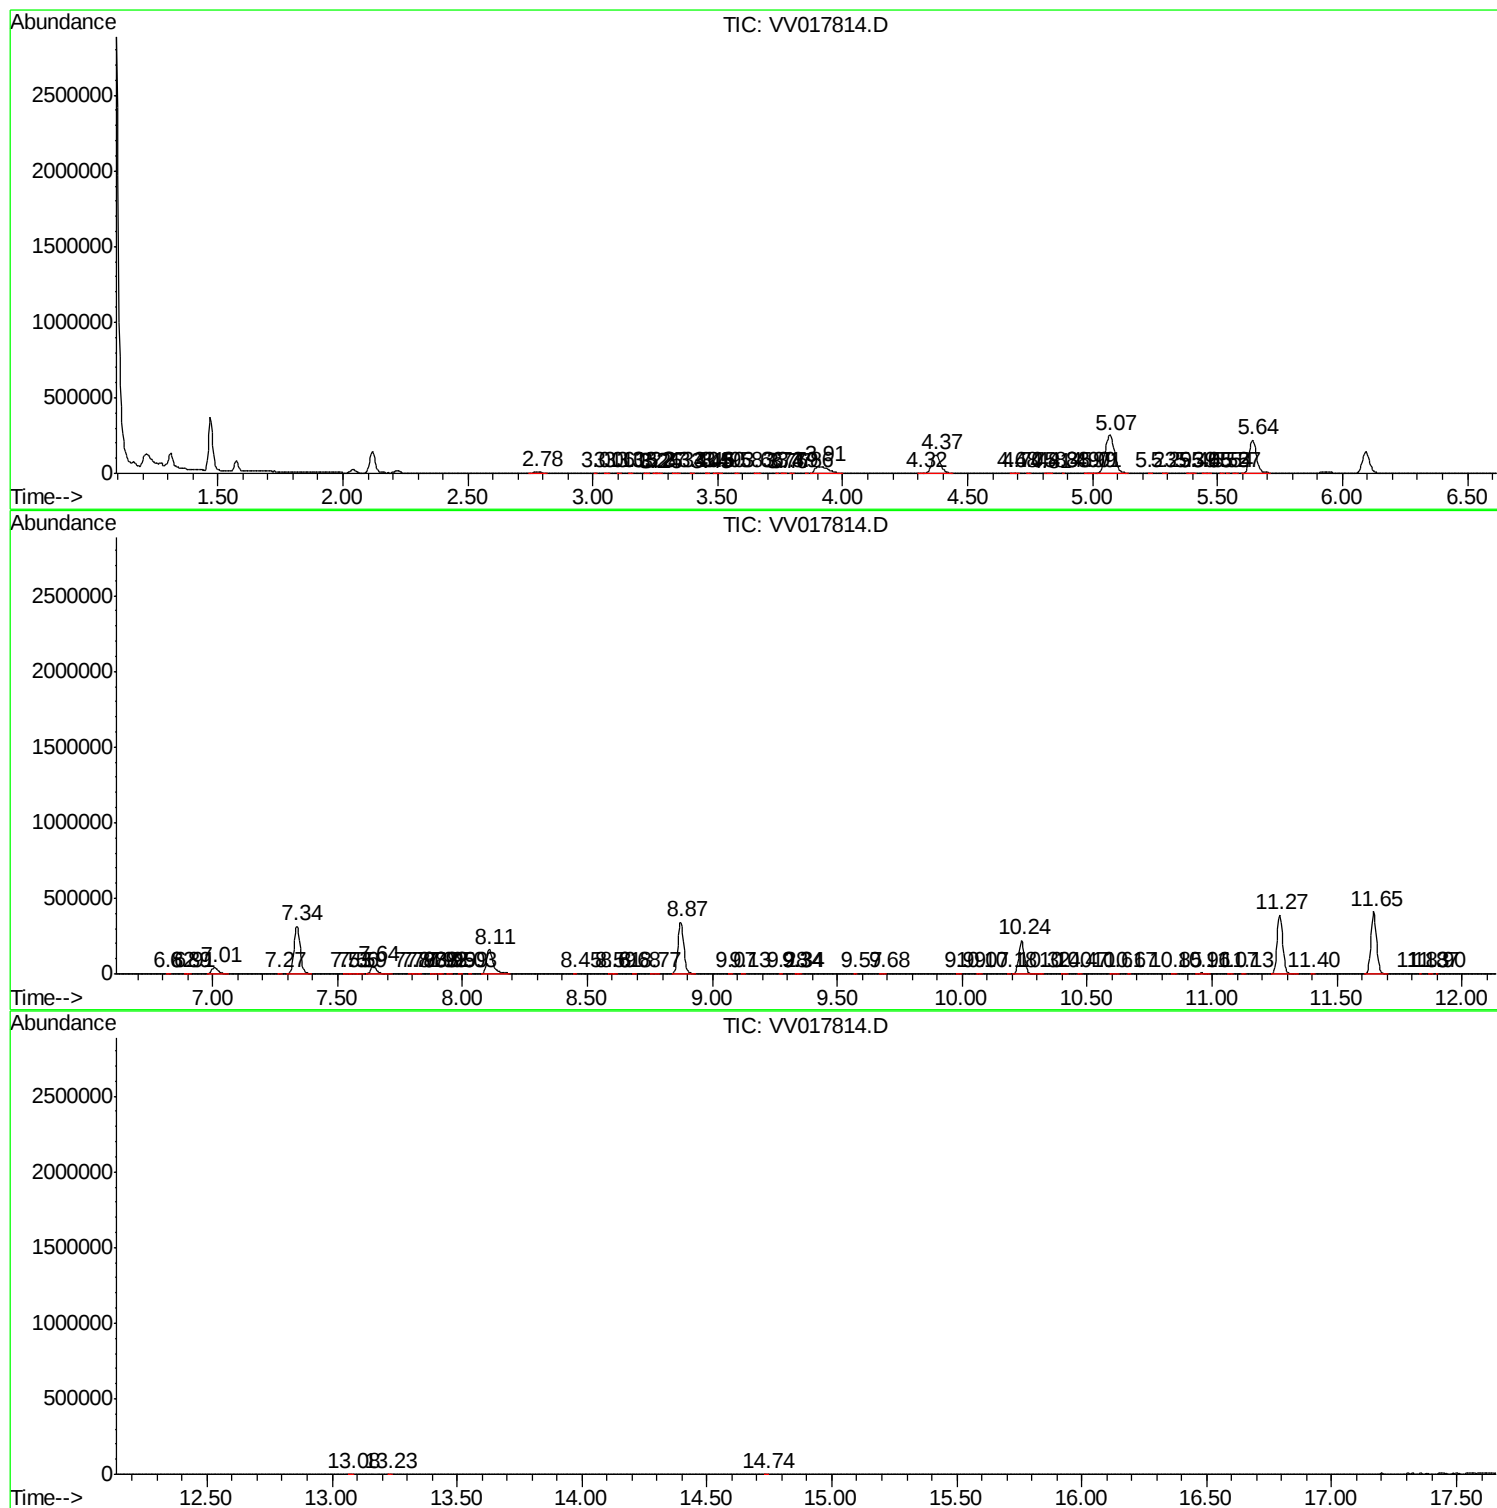

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV080620\
Data File : VV017814.D
Acq On : 06 Aug 2020 15:13
Operator : SY/MD
Sample : L3590-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F2L53

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM073020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV080620\
Data File : VV017814.D
Acq On : 06 Aug 2020 15:13
Operator : SY/MD
Sample : L3590-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F2L53

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM073020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc