

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV080620\
 Data File : VV017823.D
 Acq On : 06 Aug 2020 19:30
 Operator : SY/MD
 Sample : L3590-18
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4L24

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM073020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.299	372	376	377	rBV	775	412	0.06%	0.007%
2	2.438	415	419	421	rBV	452	323	0.04%	0.005%
3	2.550	452	454	459	rVB2	371	291	0.04%	0.005%
4	2.576	460	462	465	rBV	293	177	0.02%	0.003%
5	2.608	469	472	473	rBB	548	219	0.03%	0.004%
6	2.631	476	479	480	rBV2	424	231	0.03%	0.004%
7	2.672	490	492	494	rBV	256	160	0.02%	0.003%
8	2.688	494	497	499	rVB2	416	213	0.03%	0.004%
9	2.717	503	506	508	rBB	270	151	0.02%	0.003%
10	2.733	509	511	515	rBV	208	189	0.03%	0.003%
11	2.782	515	526	538	rBV2	21963	39208	5.31%	0.655%
12	2.843	543	545	547	rBV	267	148	0.02%	0.002%
13	2.968	582	584	587	rVB	559	266	0.04%	0.004%
14	2.994	588	592	597	rBV3	383	449	0.06%	0.007%
15	3.097	619	624	627	rBB3	273	289	0.04%	0.005%
16	3.123	627	632	635	rBB2	397	300	0.04%	0.005%
17	3.148	636	640	642	rBV	494	263	0.04%	0.004%
18	3.238	664	668	672	rBB	174	166	0.02%	0.003%
19	3.267	673	677	679	rBB	441	296	0.04%	0.005%
20	3.283	680	682	683	rBV	345	157	0.02%	0.003%
21	3.344	699	701	704	rVB	451	157	0.02%	0.003%
22	3.377	705	711	714	rBV2	437	448	0.06%	0.007%
23	3.624	786	788	790	rBV	445	195	0.03%	0.003%
24	3.637	790	792	795	rVB2	269	148	0.02%	0.002%
25	3.659	796	799	800	rBV	393	204	0.03%	0.003%
26	3.775	834	835	837	rBV	320	152	0.02%	0.003%
27	3.859	856	861	864	rBV	152	175	0.02%	0.003%
28	3.939	865	886	905	rBV4	67012	262718	35.60%	4.386%
29	4.376	1005	1022	1047	rBV	135466	334278	45.30%	5.581%
30	4.627	1096	1100	1105	rVB2	487	466	0.06%	0.008%
31	4.656	1105	1109	1112	rBV2	401	294	0.04%	0.005%
32	4.769	1140	1144	1147	rBB2	585	312	0.04%	0.005%
33	5.007	1217	1218	1220	rBV	357	172	0.02%	0.003%
34	5.071	1220	1238	1266	rBV3	284704	737999	100.00%	12.321%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV080620\
 Data File : VV017823.D
 Acq On : 06 Aug 2020 19:30
 Operator : SY/MD
 Sample : L3590-18
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4L24

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM073020WMA.M
 Title : VOC Analysis

35	5.322	1312	1316	1319	rVB3	616	469	0.06%	0.008%
36	5.348	1320	1324	1328	rBV3	597	446	0.06%	0.007%
37	5.434	1348	1351	1353	rBV3	351	233	0.03%	0.004%
38	5.556	1387	1389	1391	rBV	407	227	0.03%	0.004%
39	5.640	1402	1415	1435	rBV	270069	537417	72.82%	8.972%
40	5.823	1470	1472	1474	rBV	365	152	0.02%	0.003%
41	5.868	1485	1486	1488	rBV	348	169	0.02%	0.003%
42	5.939	1496	1508	1521	rBV	8021	17737	2.40%	0.296%
43	6.093	1543	1556	1576	rBV	163509	326478	44.24%	5.451%
44	6.248	1601	1604	1606	rBV3	489	285	0.04%	0.005%
45	6.412	1652	1655	1656	rBV2	356	181	0.02%	0.003%
46	6.454	1665	1668	1671	rBV	380	273	0.04%	0.005%
47	6.547	1695	1697	1699	rBV	357	193	0.03%	0.003%
48	6.630	1720	1723	1724	rBV	760	363	0.05%	0.006%
49	6.798	1771	1775	1777	rBV	199	186	0.03%	0.003%
50	6.814	1778	1780	1784	rVB2	500	297	0.04%	0.005%
51	6.891	1801	1804	1805	rBV	273	154	0.02%	0.003%
52	7.007	1829	1840	1859	rBV2	90065	162835	22.06%	2.719%
53	7.219	1904	1906	1908	rBV	730	321	0.04%	0.005%
54	7.277	1922	1924	1926	rBV	342	187	0.03%	0.003%
55	7.338	1931	1943	1963	rBV	358893	611614	82.87%	10.211%
56	7.566	2010	2014	2017	rBV	616	451	0.06%	0.008%
57	7.640	2027	2037	2055	rBV2	63579	109752	14.87%	1.832%
58	7.775	2077	2079	2081	rBV	378	196	0.03%	0.003%
59	7.817	2090	2092	2095	rBV	342	211	0.03%	0.004%
60	7.865	2105	2107	2109	rBV2	417	241	0.03%	0.004%
61	8.035	2158	2160	2163	rBV	273	166	0.02%	0.003%
62	8.052	2163	2165	2172	rVB2	470	287	0.04%	0.005%
63	8.106	2172	2182	2214	rBV	180412	321419	43.55%	5.366%
64	8.412	2275	2277	2282	rVB2	370	171	0.02%	0.003%
65	8.486	2296	2300	2301	rBV	310	213	0.03%	0.004%
66	8.534	2311	2315	2319	rVB	416	312	0.04%	0.005%
67	8.659	2350	2354	2355	rBV2	332	213	0.03%	0.004%
68	8.736	2374	2378	2381	rBB	484	304	0.04%	0.005%
69	8.871	2409	2420	2445	rBV	414374	668881	90.63%	11.167%
70	9.000	2458	2460	2463	rVB2	696	356	0.05%	0.006%
71	9.116	2492	2496	2498	rBV2	372	243	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV080620\
 Data File : VV017823.D
 Acq On : 06 Aug 2020 19:30
 Operator : SY/MD
 Sample : L3590-18
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4L24

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM073020WMA.M
 Title : VOC Analysis

72	9.161	2505	2510	2511	rBV2	522	361	0.05%	0.006%
73	9.235	2530	2533	2537	rBV	346	285	0.04%	0.005%
74	9.338	2562	2565	2569	rBB	282	245	0.03%	0.004%
75	9.405	2582	2586	2590	rBB	366	224	0.03%	0.004%
76	9.428	2591	2593	2595	rBV	283	176	0.02%	0.003%
77	9.736	2686	2689	2693	rVB2	418	282	0.04%	0.005%
78	9.775	2698	2701	2708	rBV2	595	536	0.07%	0.009%
79	9.900	2737	2740	2743	rBV2	448	417	0.06%	0.007%
80	10.122	2807	2809	2814	rBV	402	339	0.05%	0.006%
81	10.235	2833	2844	2861	rBV	243936	381051	51.63%	6.362%
82	10.383	2888	2890	2893	rBV2	370	210	0.03%	0.004%
83	10.633	2964	2968	2971	rBV	453	350	0.05%	0.006%
84	10.736	2998	3000	3002	rBV2	366	177	0.02%	0.003%
85	10.955	3067	3068	3072	rBV	271	164	0.02%	0.003%
86	11.032	3086	3092	3093	rBV	348	331	0.04%	0.006%
87	11.100	3106	3113	3116	rBB	469	392	0.05%	0.007%
88	11.119	3116	3119	3122	rBV	318	280	0.04%	0.005%
89	11.270	3155	3166	3190	rBV	487097	737196	99.89%	12.308%
90	11.489	3230	3234	3235	rBV	458	319	0.04%	0.005%
91	11.646	3270	3283	3302	rBV	464855	718878	97.41%	12.002%
92	12.077	3415	3417	3421	rBV	372	232	0.03%	0.004%
93	12.215	3456	3460	3461	rBV	263	162	0.02%	0.003%
94	12.357	3502	3504	3505	rBV	482	174	0.02%	0.003%
95	12.524	3554	3556	3557	rBV	380	181	0.02%	0.003%
96	12.704	3608	3612	3613	rBV	351	222	0.03%	0.004%
97	12.756	3626	3628	3632	rBV	372	213	0.03%	0.004%
98	13.537	3868	3871	3875	rBV	563	434	0.06%	0.007%
99	13.801	3949	3953	3958	rBV	375	403	0.05%	0.007%
100	13.961	4002	4003	4005	rBV2	579	194	0.03%	0.003%


Sum of corrected areas: 5989687

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV080620\
Data File : VV017823.D
Acq On : 06 Aug 2020 19:30
Operator : SY/MD
Sample : L3590-18
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4L24

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM073020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

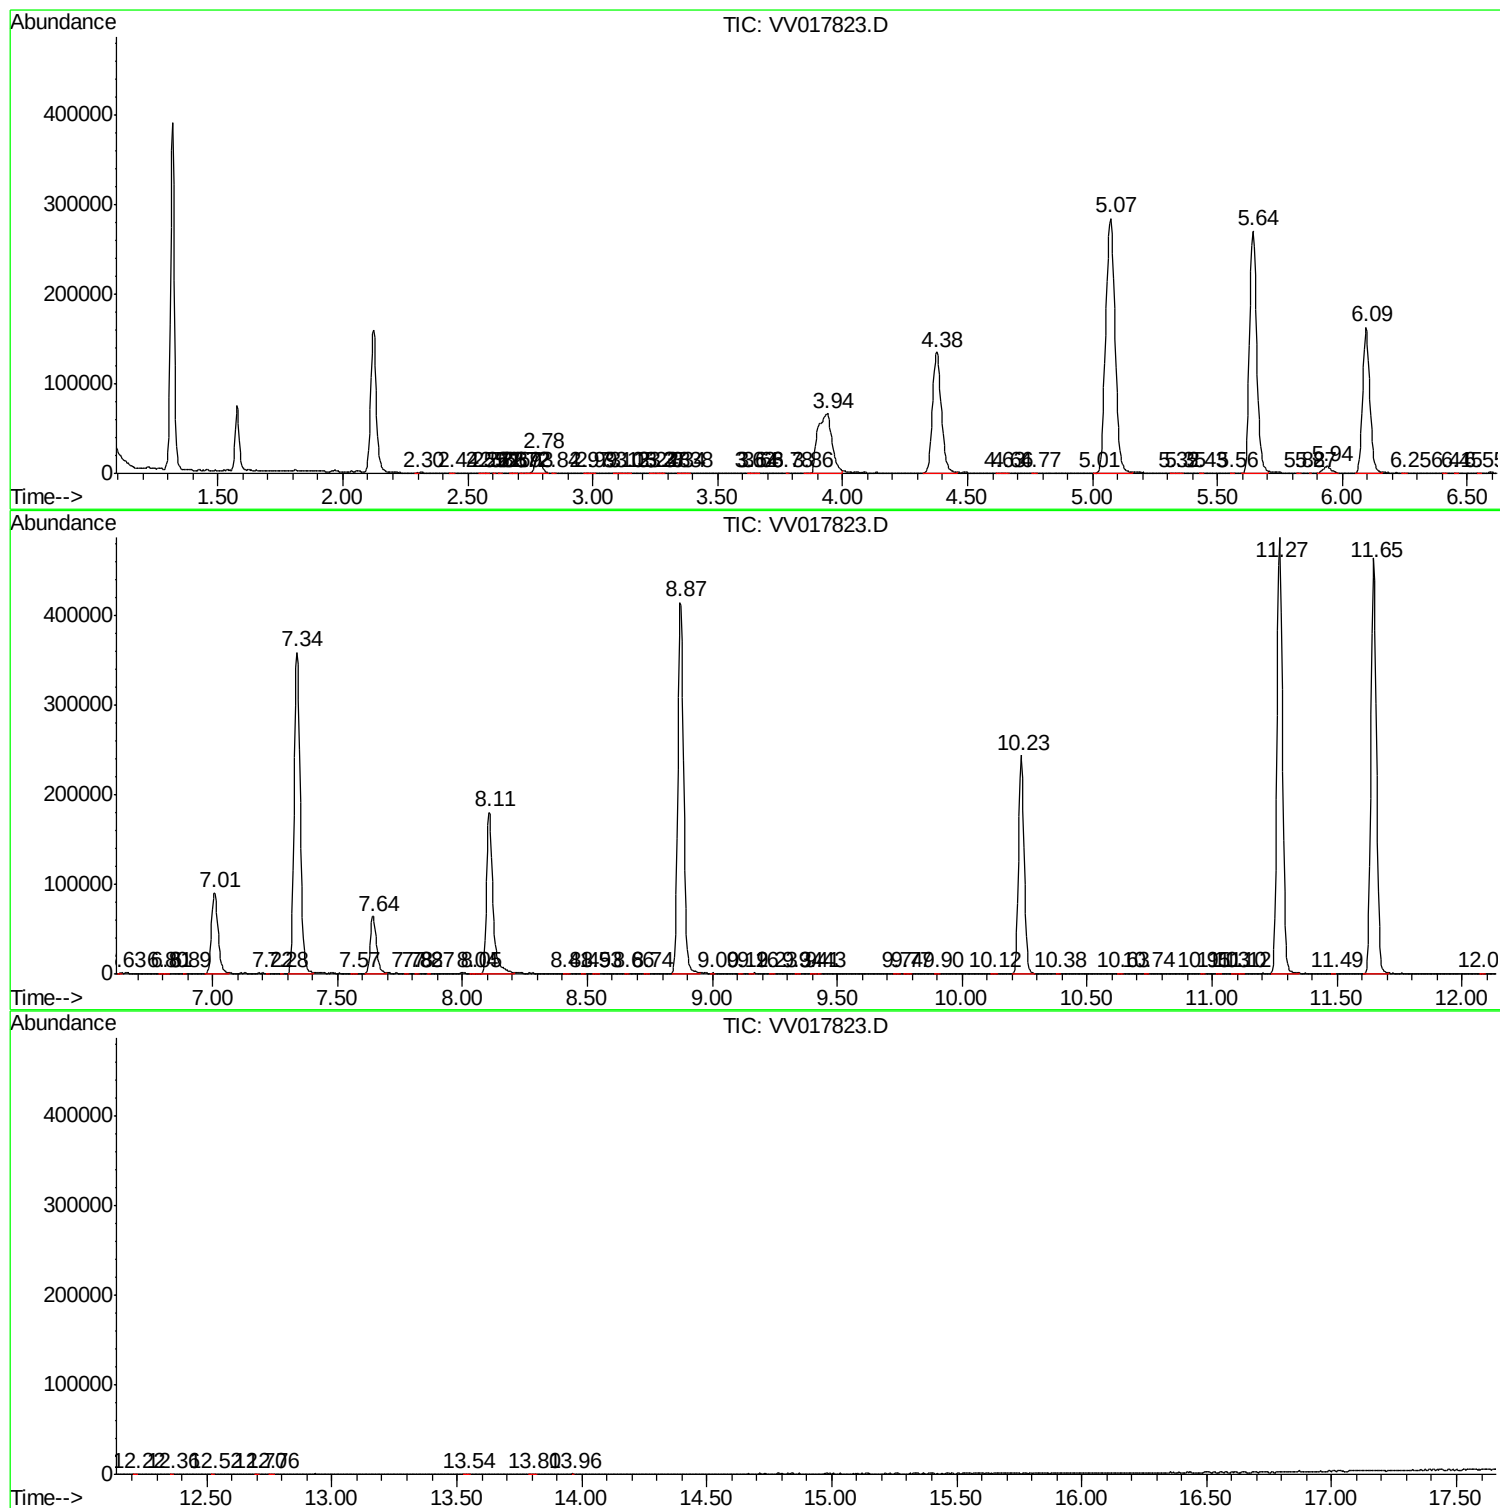

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV080620\
Data File : VV017823.D
Acq On : 06 Aug 2020 19:30
Operator : SY/MD
Sample : L3590-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4L24

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM073020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV080620\
Data File : VV017823.D
Acq On : 06 Aug 2020 19:30
Operator : SY/MD
Sample : L3590-18
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
F4L24

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM073020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc