


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV080620\
 Data File : VV017802.D
 Acq On : 06 Aug 2020 08:54
 Operator : SY/MD
 Sample : BFB67
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB67

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM073020WMA.M
 Title : VOC Analysis
 Last Update : Fri Aug 07 05:27:52 2020

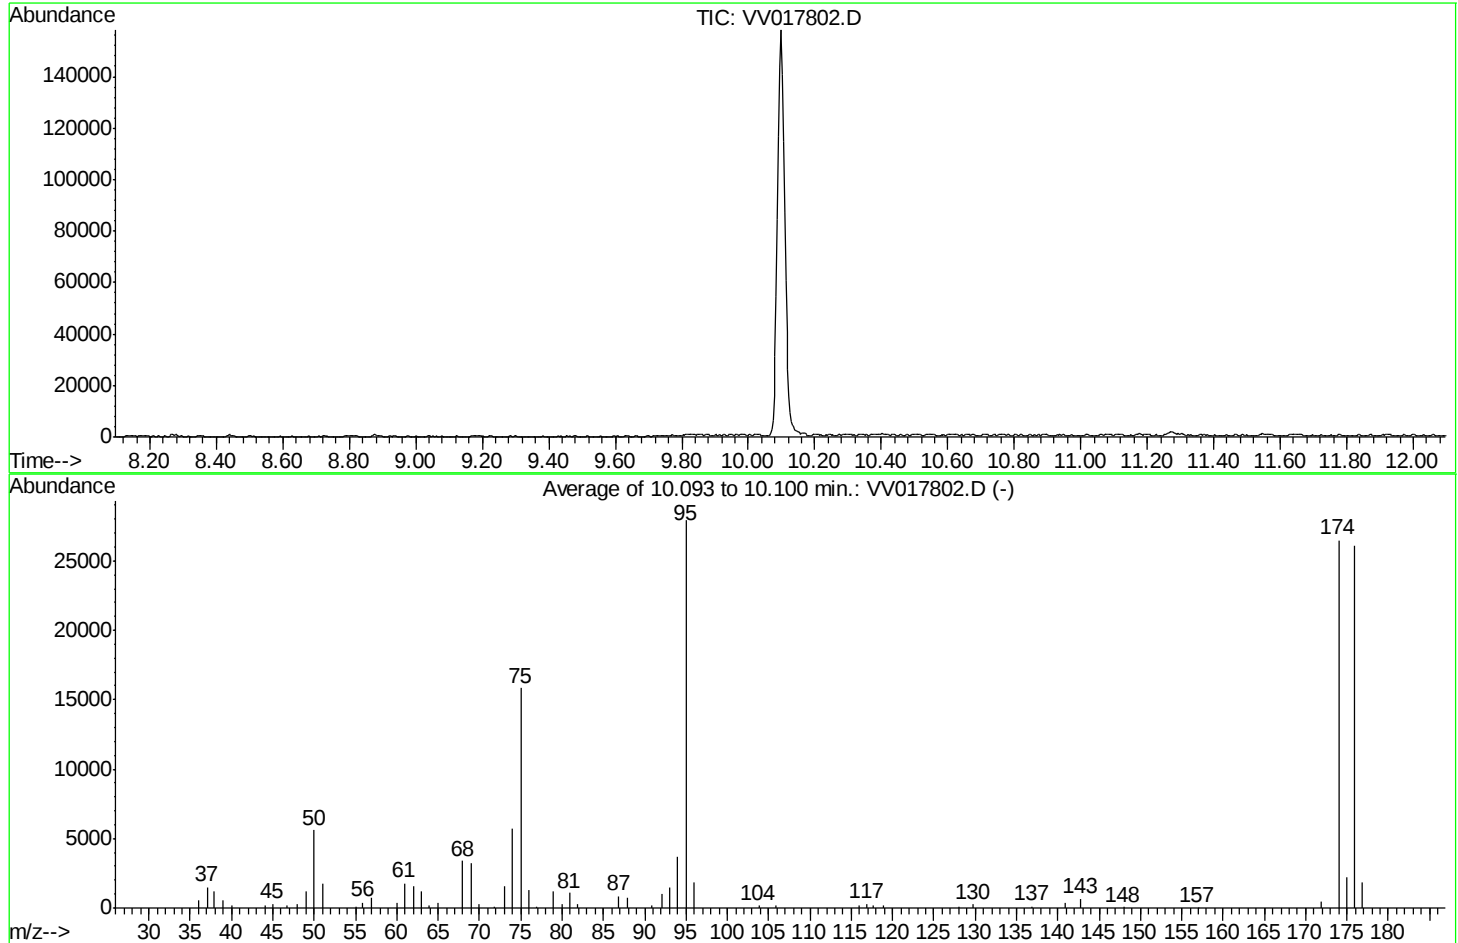

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2790

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	5606	PASS
75	95	30	80	56.7	15844	PASS
95	95	100	100	100.0	27920	PASS
96	95	5	9	6.5	1805	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	94.9	26488	PASS
175	174	5	9	8.3	2194	PASS
176	174	95	101	98.5	26093	PASS
177	176	5	9	7.2	1886	PASS

m/z	Abundance
36.00	850.0
37.00	1401.0
38.00	1288.0
39.00	565.0
40.00	164.0
44.00	244.0
45.00	326.0
46.80	156.0
47.90	238.0
49.00	1095.0
50.00	5269.0
51.10	1715.0
55.10	113.0
55.90	412.0
57.00	771.0
59.90	364.0
61.00	1709.0
62.00	1492.0
63.00	1174.0
63.90	243.0
65.00	430.0
68.00	3101.0
69.00	3056.0
69.90	229.0
71.80	138.0
73.00	1308.0
74.00	5470.0
75.00	15190.0
76.00	1279.0
76.80	110.0
78.90	1109.0
79.90	270.0
80.90	1090.0
81.90	235.0
86.80	809.0
87.80	675.0
90.80	184.0
92.10	970.0
92.90	1386.0
94.00	3436.0
95.00	26384.0
96.00	1778.0
103.80	151.0
105.90	103.0
115.90	201.0
116.90	274.0
117.80	152.0
119.00	175.0
128.00	119.0
129.80	226.0
136.90	158.0
140.90	330.0
142.80	581.0
148.00	120.0
171.80	404.0
174.00	24632.0
174.90	2109.0
175.90	24256.0
176.90	1637.0

Instrument :
MSVOA_V
ClientSampleId :
BFB67

m/z	Abundance
36.00	839.0
37.00	1534.0
38.00	1431.0
39.00	595.0
40.00	212.0
44.00	310.0
45.00	321.0
46.80	160.0
47.90	291.0
49.00	1268.0
50.00	5840.0
51.00	1794.0
55.80	411.0
57.00	823.0
60.00	406.0
60.90	1857.0
62.00	1572.0
63.00	1186.0
63.90	235.0
65.00	408.0
68.00	3608.0
69.00	3337.0
69.90	310.0
71.80	144.0
73.00	1615.0
74.00	5909.0
75.00	16392.0
75.90	1301.0
76.80	141.0
78.90	1255.0
80.00	281.0
80.90	1105.0
81.90	243.0
86.90	815.0
87.90	815.0
90.80	180.0
92.00	1001.0
93.00	1572.0
94.00	3851.0
95.00	28960.0
96.00	1902.0
103.80	170.0
106.00	172.0
115.90	201.0
116.90	295.0
117.70	176.0
118.90	184.0
128.00	131.0
129.80	264.0
136.90	146.0
140.80	360.0
142.80	671.0
148.00	113.0
157.00	100.0
171.90	419.0
174.00	27416.0
175.00	2262.0
175.90	26880.0
176.90	1963.0

Instrument :
MSVOA_V
ClientSampleId :
BFB67

m/z	Abundance
36.00	743.0
37.10	1541.0
38.00	1479.0
39.00	598.0
40.00	191.0
44.00	332.0
44.90	302.0
46.70	121.0
47.90	275.0
49.00	1269.0
50.00	5709.0
51.00	1717.0
55.10	118.0
55.90	399.0
57.00	747.0
60.10	371.0
60.90	1713.0
62.00	1533.0
63.00	1226.0
63.90	196.0
65.00	369.0
68.00	3476.0
69.00	3244.0
69.90	324.0
71.90	124.0
73.00	1689.0
74.00	5715.0
75.00	15951.0
76.00	1225.0
76.90	147.0
78.90	1355.0
80.00	309.0
80.90	1038.0
81.90	242.0
87.00	917.0
87.90	864.0
90.80	149.0
92.00	976.0
93.00	1528.0
94.00	3862.0
95.00	28416.0
96.00	1736.0
103.80	143.0
106.00	180.0
116.00	171.0
116.90	287.0
117.60	226.0
119.00	178.0
128.00	150.0
129.80	215.0
140.90	370.0
142.80	738.0
172.00	452.0
174.00	27416.0
174.90	2211.0
176.00	27144.0
176.90	2060.0

Instrument :
MSVOA_V
ClientSampleId :
BFB67

Scan 2790 (10.061 min): VV017802.D
BFB67

m/z	Abundance
35.90	283.0
37.90	177.0
44.10	138.0

Instrument :
MSVOA_V
ClientSampleId :
BFB67