

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080621\
 Data File : VV021746.D
 Acq On : 06 Aug 2021 10:36
 Operator : SY/MD
 Sample : VV0806MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK226

Quant Time: Aug 07 01:49:49 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080221WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Aug 07 01:48:22 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	401658	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	374011	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	180876	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	106126	42.073	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	84.140%		
7) Chloroethane-d5	1.564	69	93846	45.110	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	90.220%		
11) 1,1-Dichloroethene-d2	2.105	63	145400	32.229	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	64.460%		
21) 2-Butanone-d5	3.880	46	220143	101.600	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	101.600%		
24) Chloroform-d	4.346	84	250423	46.839	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.680%		
26) 1,2-Dichloroethane-d4	5.031	65	154752	48.400	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	96.800%		
32) Benzene-d6	5.047	84	521697	49.214	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	98.420%		
36) 1,2-Dichloropropane-d6	6.069	67	167375	49.815	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	99.640%		
41) Toluene-d8	7.317	98	479577	48.897	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	97.800%		
43) trans-1,3-Dichloroprop...	7.622	79	78826	47.546	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	95.100%		
47) 2-Hexanone-d5	8.088	63	132125	90.184	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	90.180%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	196615	44.401	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	88.800%		
66) 1,2-Dichlorobenzene-d4	11.625	152	187299	50.013	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	100.020%		
Target Compounds					Qvalue	
48) 2-Hexanone	8.143	43	16800	5.614	ug/L	# 86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080621\
Data File : VV021746.D
Acq On : 06 Aug 2021 10:36
Operator : SY/MD
Sample : VV0806MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK226


Quant Time: Aug 07 01:49:49 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080221WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Aug 07 01:48:22 2021
Response via : Initial Calibration

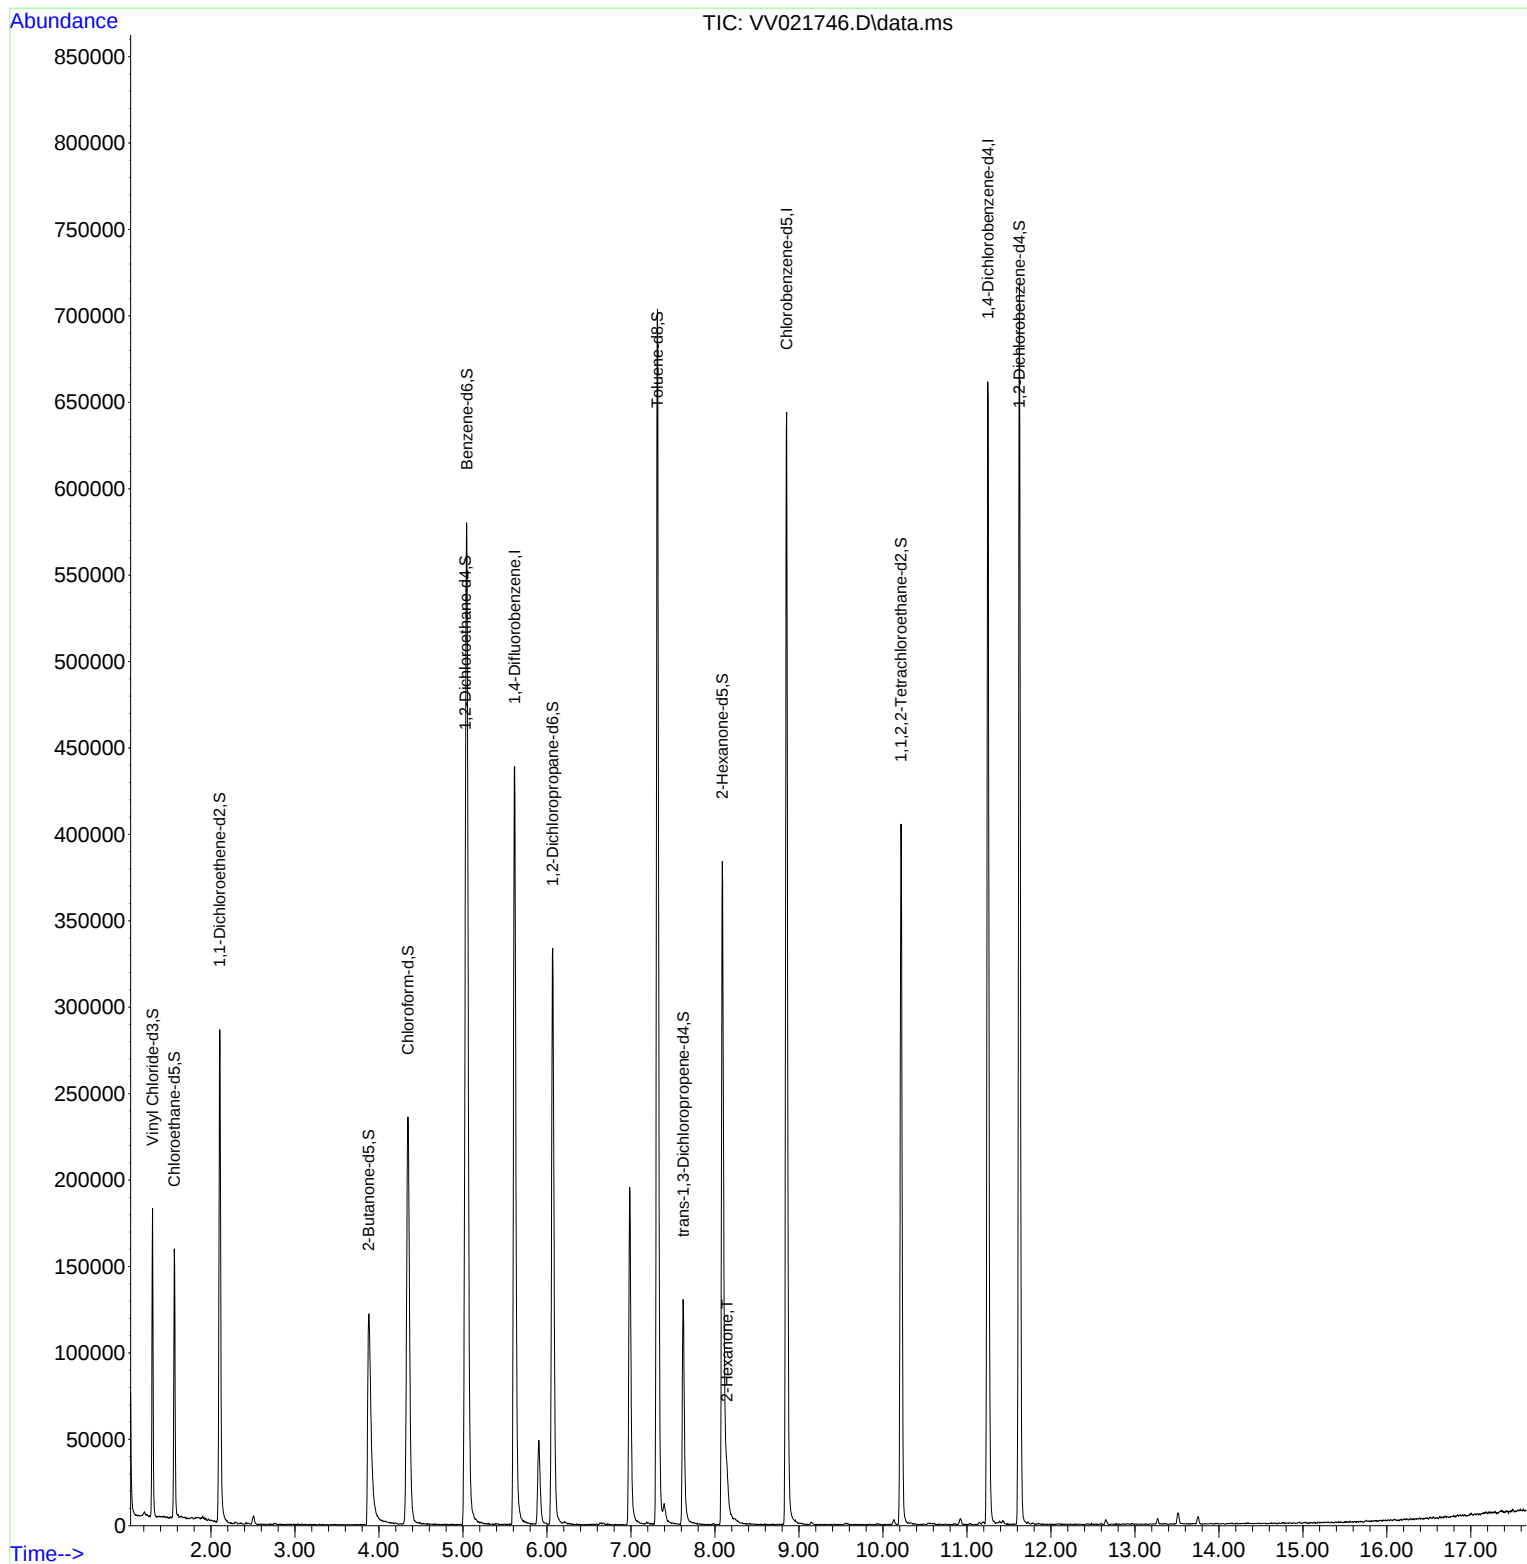

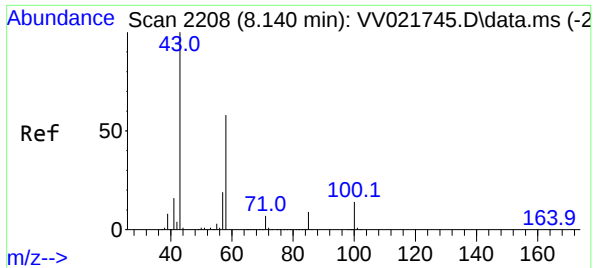

#48
2-Hexanone
Concen: 5.614 ug/L
RT: 8.143 min Scan# 2209
Delta R.T. 0.003 min
Lab File: VV021746.D
Acq: 06 Aug 2021 10:36

Instrument :
MSVOA_V
ClientSampleId :
VBLK226

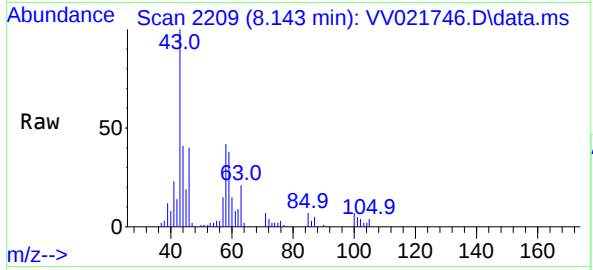

Tgt Ion: 43 Resp: 16800

Ion	Ratio	Lower	Upper
43	100		
58	46.1	46.0	69.0
57	15.3	15.0	22.4
100	8.0	11.1	16.7#

