

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080621\
 Data File : VV021747.D
 Acq On : 06 Aug 2021 11:02
 Operator : SY/MD
 Sample : VV0806WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK227

Quant Time: Aug 07 01:50:01 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080221WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Aug 07 01:48:22 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	385908	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	358790	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	172228	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	101345	41.817	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	83.640%
7) Chloroethane-d5	1.561	69	79568	39.808	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	79.620%
11) 1,1-Dichloroethene-d2	2.105	63	142107	32.784	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	65.560%
21) 2-Butanone-d5	3.876	46	216247	103.875	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	103.870%
24) Chloroform-d	4.346	84	243759	47.453	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.900%
26) 1,2-Dichloroethane-d4	5.031	65	152435	49.621	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.240%
32) Benzene-d6	5.050	84	506458	49.803	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.600%
36) 1,2-Dichloropropane-d6	6.069	67	163259	50.651	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	101.300%
41) Toluene-d8	7.317	98	461597	49.060	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	98.120%
43) trans-1,3-Dichloroprop...	7.622	79	75524	47.487	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	94.980%
47) 2-Hexanone-d5	8.088	63	132910	94.568	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	94.570%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	193006	45.435	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	90.880%
66) 1,2-Dichlorobenzene-d4	11.625	152	182199	51.094	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	102.180%
Target Compounds						
					Qvalue	
48) 2-Hexanone	8.143	43	15992	5.571	ug/L	# 85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080621\
Data File : VV021747.D
Acq On : 06 Aug 2021 11:02
Operator : SY/MD
Sample : VV0806WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK227

Quant Time: Aug 07 01:50:01 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080221WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Aug 07 01:48:22 2021
Response via : Initial Calibration

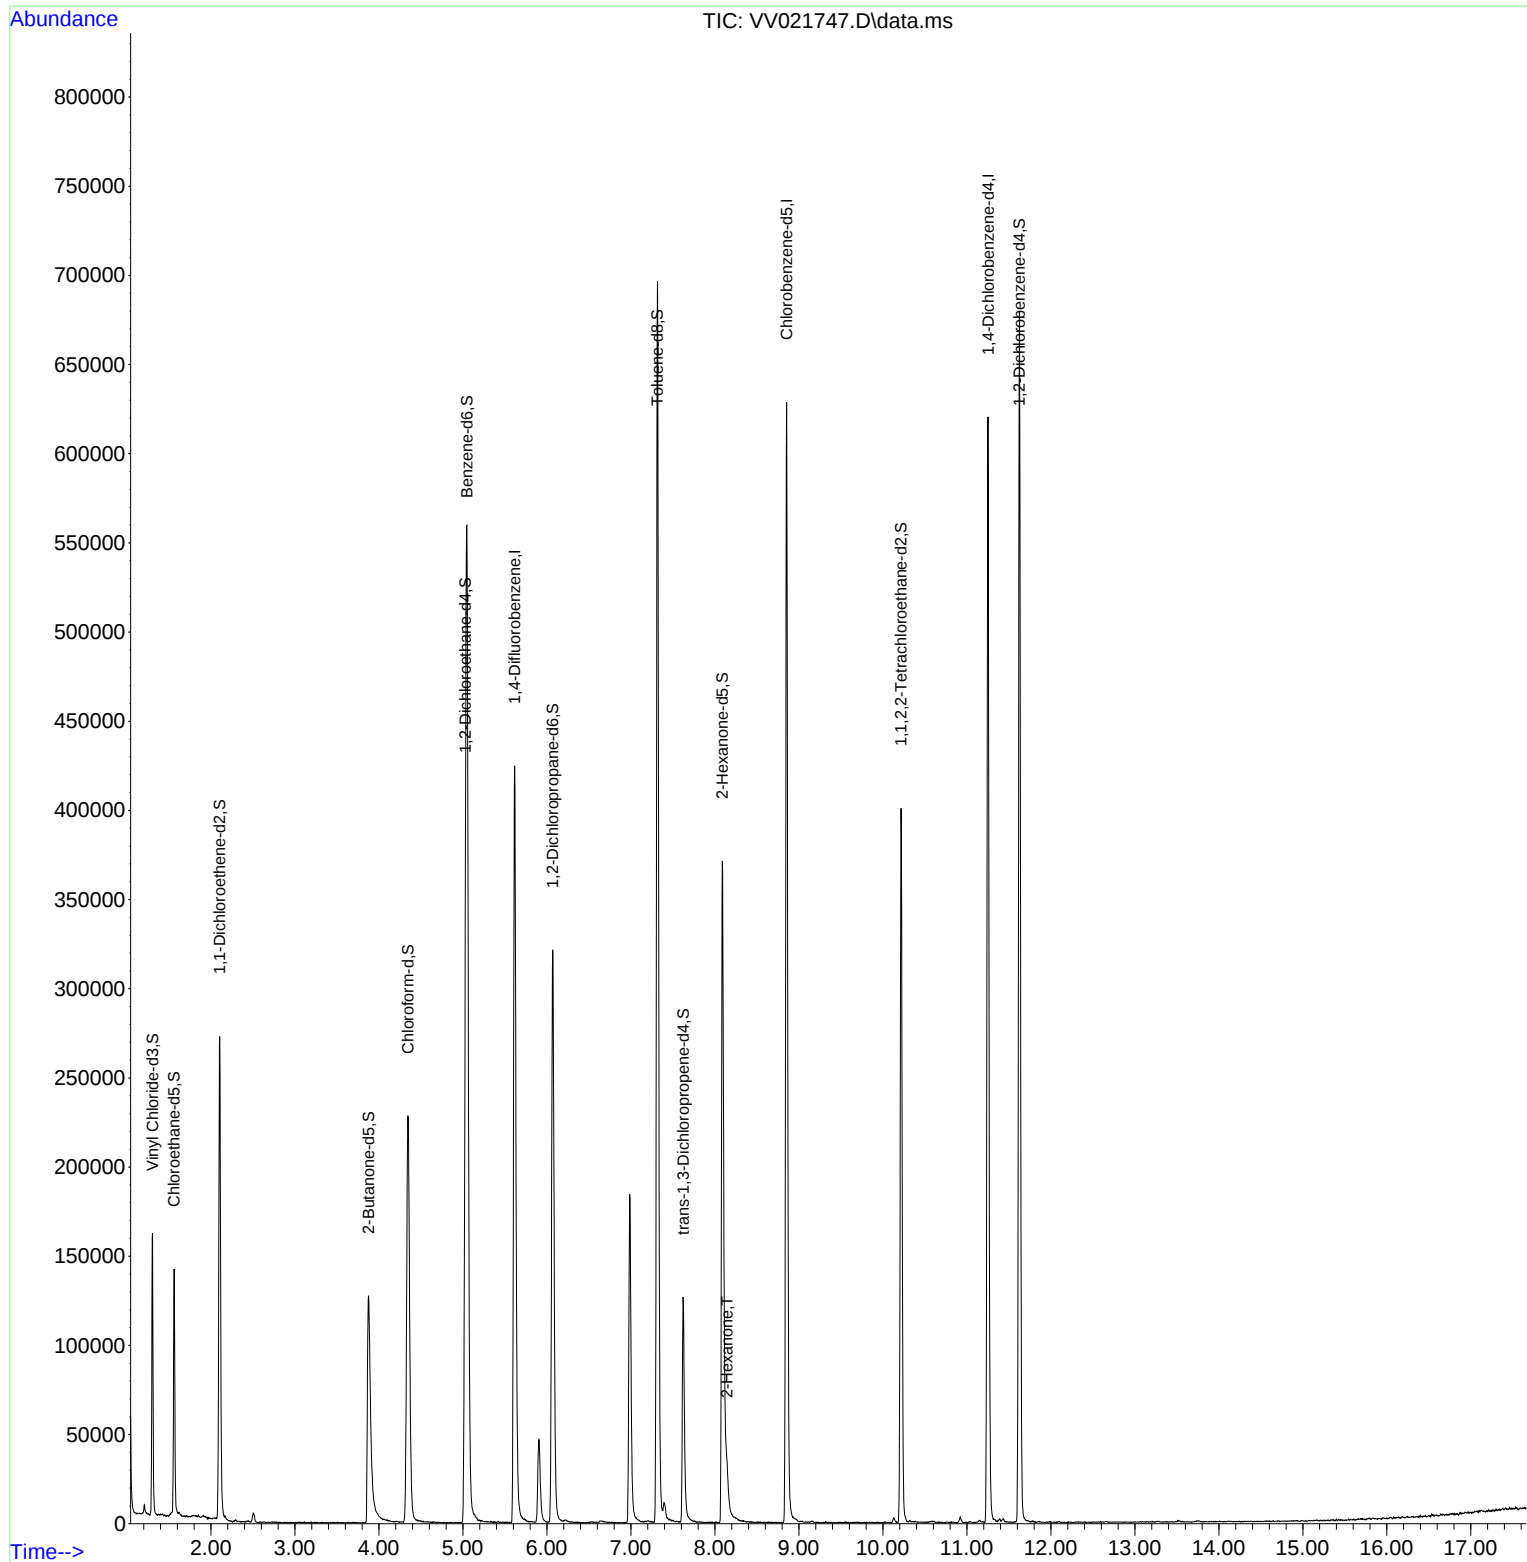

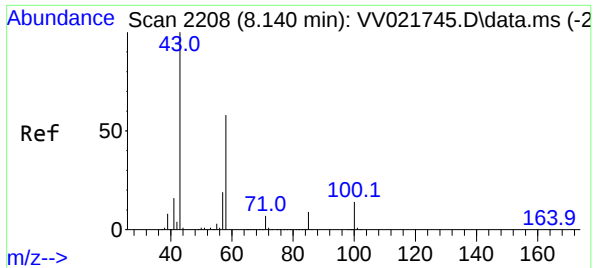

#48
2-Hexanone
Concen: 5.571 ug/L
RT: 8.143 min Scan# 2209
Delta R.T. 0.003 min
Lab File: VV021747.D
Acq: 06 Aug 2021 11:02

Instrument :
MSVOA_V
ClientSampleId :
VBLK227

Tgt Ion: 43 Resp: 15992

Ion	Ratio	Lower	Upper
43	100		
58	44.6	46.0	69.0#
57	19.2	15.0	22.4
100	4.4	11.1	16.7#

