


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080621\
 Data File : VV021744.D
 Acq On : 06 Aug 2021 09:35
 Operator : SY/MD
 Sample : BFB213
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB213

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080221WMA.M
 Title : VOC Analysis
 Last Update : Tue Aug 10 01:21:22 2021

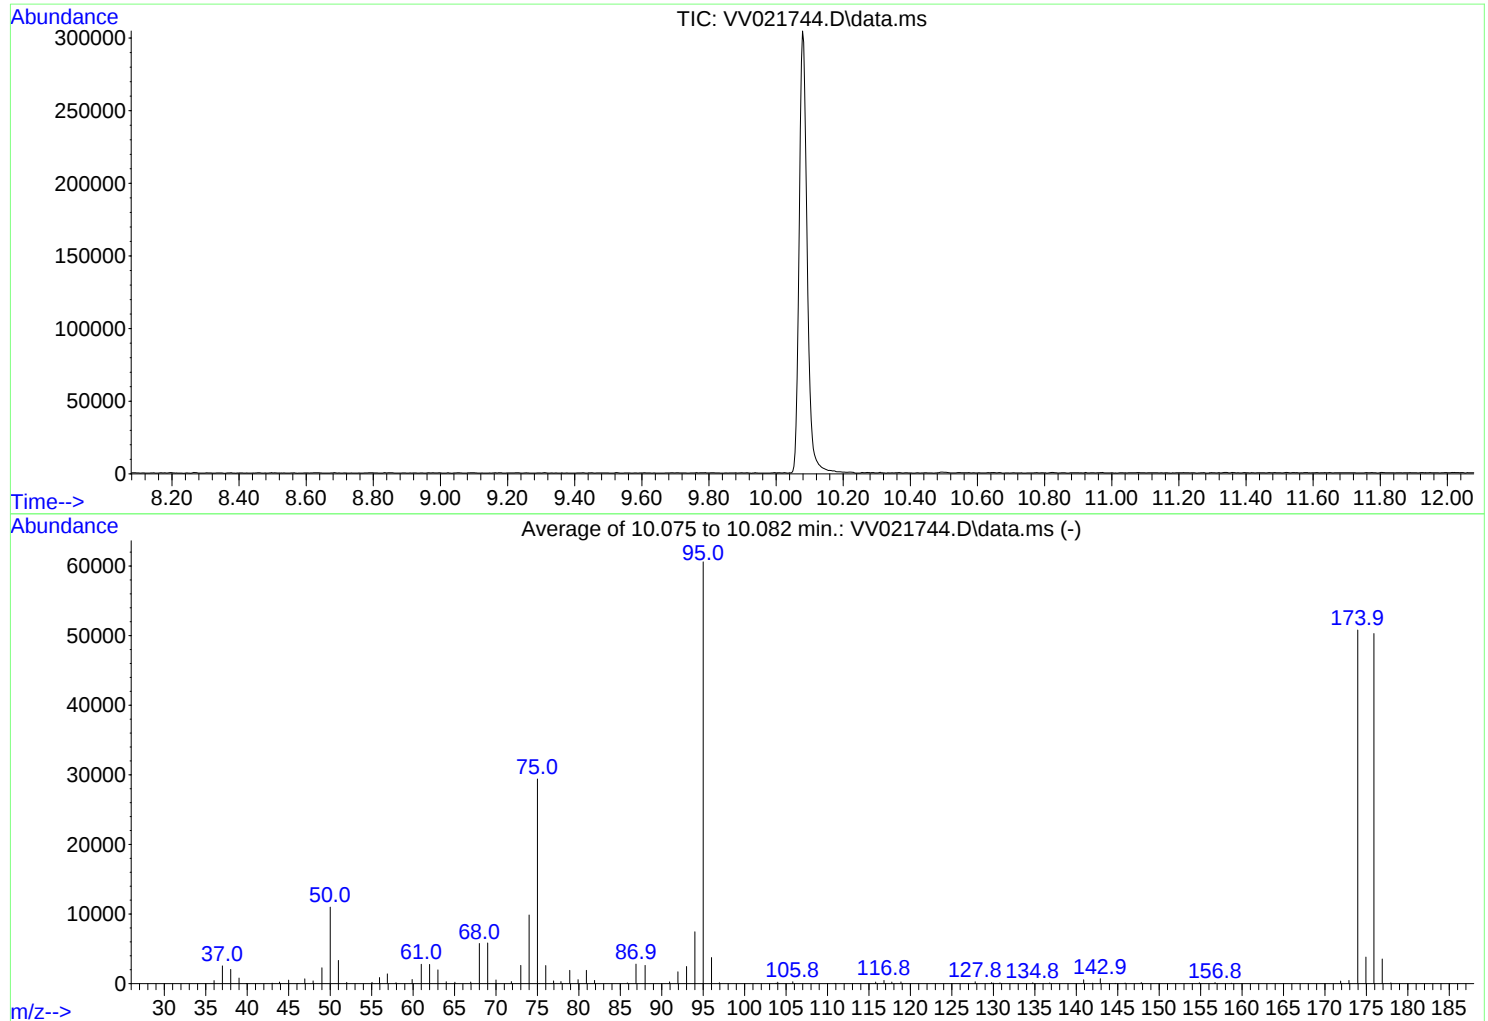

AutoFind: Scans 2810, 2811, 2812; Background Corrected with Scan 2799

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	10983	PASS
75	95	30	80	48.5	29416	PASS
95	95	100	100	100.0	60608	PASS
96	95	5	9	6.2	3749	PASS
173	174	0.00	2	0.9	471	PASS
174	95	50	120	83.8	50808	PASS
175	174	5	9	7.5	3813	PASS
176	174	95	105	99.0	50315	PASS
177	176	5	10	7.1	3550	PASS

m/z	Abundance
36.00	444.0
37.00	2667.0
38.00	2121.0
39.00	793.0
39.90	148.0
43.00	111.0
44.00	759.0
45.00	497.0
47.00	684.0
47.90	416.0
49.00	2386.0
50.00	11310.0
51.00	3491.0
52.00	189.0
55.00	193.0
55.90	900.0
56.90	1459.0
58.00	126.0
59.90	624.0
61.00	2820.0
62.00	2852.0
63.00	2022.0
64.00	309.0
65.10	204.0
66.90	212.0
68.00	5949.0
69.00	6064.0
70.00	545.0
71.90	313.0
73.00	2698.0
74.00	10177.0
75.00	30376.0
76.00	2671.0
76.90	393.0
77.80	319.0
78.90	1976.0
79.90	570.0
80.90	1970.0
81.90	460.0
85.80	125.0
86.90	2873.0
88.00	2735.0
90.90	274.0
91.90	1752.0
93.00	2577.0
94.00	7739.0
95.00	62776.0
96.00	3861.0
97.00	136.0
104.00	273.0
105.80	298.0
115.80	237.0
116.80	498.0
117.70	237.0
118.80	271.0
127.80	294.0
129.80	234.0
130.80	121.0
134.80	145.0
136.80	133.0
140.90	570.0
142.00	106.0
142.90	746.0
145.90	133.0
147.80	174.0
154.90	147.0
156.70	165.0
158.70	105.0
171.90	413.0
172.90	489.0
173.90	52224.0
175.00	3992.0
175.90	51960.0
176.90	3721.0
178.00	132.0

Instrument :
MSVOA_V
ClientSampleId :
BFB213

m/z	Abundance
36.00	409.0
37.00	2497.0
38.00	1958.0
39.00	753.0
39.90	165.0
43.00	105.0
44.00	808.0
45.00	561.0
46.10	102.0
46.90	670.0
47.90	355.0
49.00	2323.0
50.00	10623.0
51.00	3192.0
52.00	192.0
55.00	181.0
56.00	897.0
56.90	1317.0
58.00	130.0
59.90	589.0
61.00	2634.0
62.00	2629.0
63.00	1983.0
64.00	252.0
65.10	215.0
67.00	240.0
68.00	5649.0
69.00	5719.0
70.00	504.0
71.90	285.0
73.00	2676.0
74.00	9888.0
75.00	28928.0
76.00	2603.0
77.00	339.0
77.80	272.0
78.90	1923.0
79.90	483.0
80.90	1890.0
81.90	365.0
85.90	116.0
86.90	2585.0
88.00	2655.0
91.00	294.0
92.00	1600.0
93.00	2366.0
94.00	7146.0
95.00	58208.0
96.00	3755.0
96.90	145.0
103.80	184.0
105.80	256.0
110.90	117.0
115.80	260.0
116.80	410.0
117.70	210.0
118.80	276.0
127.80	272.0
129.80	250.0
130.80	109.0
134.70	163.0
136.80	121.0
140.90	505.0
141.90	114.0
142.90	663.0
144.70	115.0
147.90	180.0
154.80	144.0
156.80	146.0
158.70	101.0
171.90	348.0
172.90	435.0
173.90	47728.0
175.00	3682.0
175.90	47168.0
176.90	3354.0
177.90	102.0

Instrument :
MSVOA_V
ClientSampleId :
BFB213

Scan 2799 (10.040 min): VV021744.D\data.ms
BFB213

m/z	Abundance
39.90	119.0
40.20	124.0
43.90	508.0

Instrument :
MSVOA_V
ClientSampleId :
BFB213

m/z	Abundance
36.00	475.0
37.00	2506.0
38.00	2046.0
39.00	872.0
40.00	149.0
43.90	664.0
45.00	455.0
47.00	706.0
48.00	405.0
49.00	2159.0
50.00	11017.0
51.00	3292.0
52.00	160.0
55.10	182.0
55.90	834.0
56.90	1469.0
57.90	138.0
59.90	579.0
61.00	2870.0
62.00	2822.0
63.00	1961.0
64.00	303.0
65.00	209.0
66.90	213.0
68.00	5719.0
69.00	5758.0
70.00	517.0
71.80	320.0
73.00	2494.0
74.00	9496.0
75.00	28944.0
76.00	2523.0
76.90	434.0
77.90	323.0
78.90	1853.0
79.90	676.0
80.90	1855.0
81.90	554.0
85.80	124.0
86.90	2965.0
88.00	2474.0
90.90	219.0
91.90	1754.0
93.00	2470.0
94.00	7480.0
95.00	60840.0
96.00	3630.0
97.00	116.0
104.00	335.0
105.80	284.0
115.80	211.0
116.80	477.0
117.80	249.0
118.90	244.0
127.80	256.0
130.00	224.0
130.80	106.0
134.80	127.0
136.80	112.0
140.90	581.0
142.90	716.0
145.90	140.0
147.80	158.0
154.90	133.0
156.70	157.0
171.90	379.0
172.90	490.0
174.00	52472.0
174.90	3766.0
175.90	51816.0
176.90	3576.0
178.00	147.0

Instrument :
MSVOA_V
ClientSampleId :
BFB213