

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV080718\
 Data File : VV006918.D
 Acq On : 08 Aug 2018 00:50
 Operator : SY/MD
 Sample : J4357-07
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ESWS6

Quant Time: Aug 08 07:43:29 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080718WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Aug 08 07:06:57 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	186215	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	176009	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	66380	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	67606	6.05	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	121.00%
7) Chloroethane-d5	1.58	69	60276	5.52	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	110.40%
11) 1,1-Dichloroethene-d2	2.13	63	93758	4.08	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	81.60%
20) 2-Butanone-d5	3.97	46	218699	61.39	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	122.78%
24) Chloroform-d	4.41	84	133627	5.70	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	114.00%
26) 1,2-Dichloroethane-d4	5.09	65	74223	5.94	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	118.80%
32) Benzene-d6	5.10	84	251566	5.84	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	116.80%
36) 1,2-Dichloropropane-d6	6.12	67	88840	5.67	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	113.40%
41) Toluene-d8	7.37	98	185780	4.98	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.60%
43) trans-1,3-Dichloropropene-	7.67	79	23856	4.72	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	94.40%
46) 2-Hexanone-d5	8.15	63	115245	54.83	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	109.66%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	68538	5.83	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	116.60%
64) 1,2-Dichlorobenzene-d4	11.68	152	64087	5.97	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	119.40%


Target Compounds					Ovalue
13) Acetone	2.21	43	9223	3.97 ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV080718\
Data File : VV006918.D
Acq On : 08 Aug 2018 00:50
Operator : SY/MD
Sample : J4357-07
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ESWS6

Quant Time: Aug 08 07:43:29 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Aug 08 07:06:57 2018
Response via : Initial Calibration

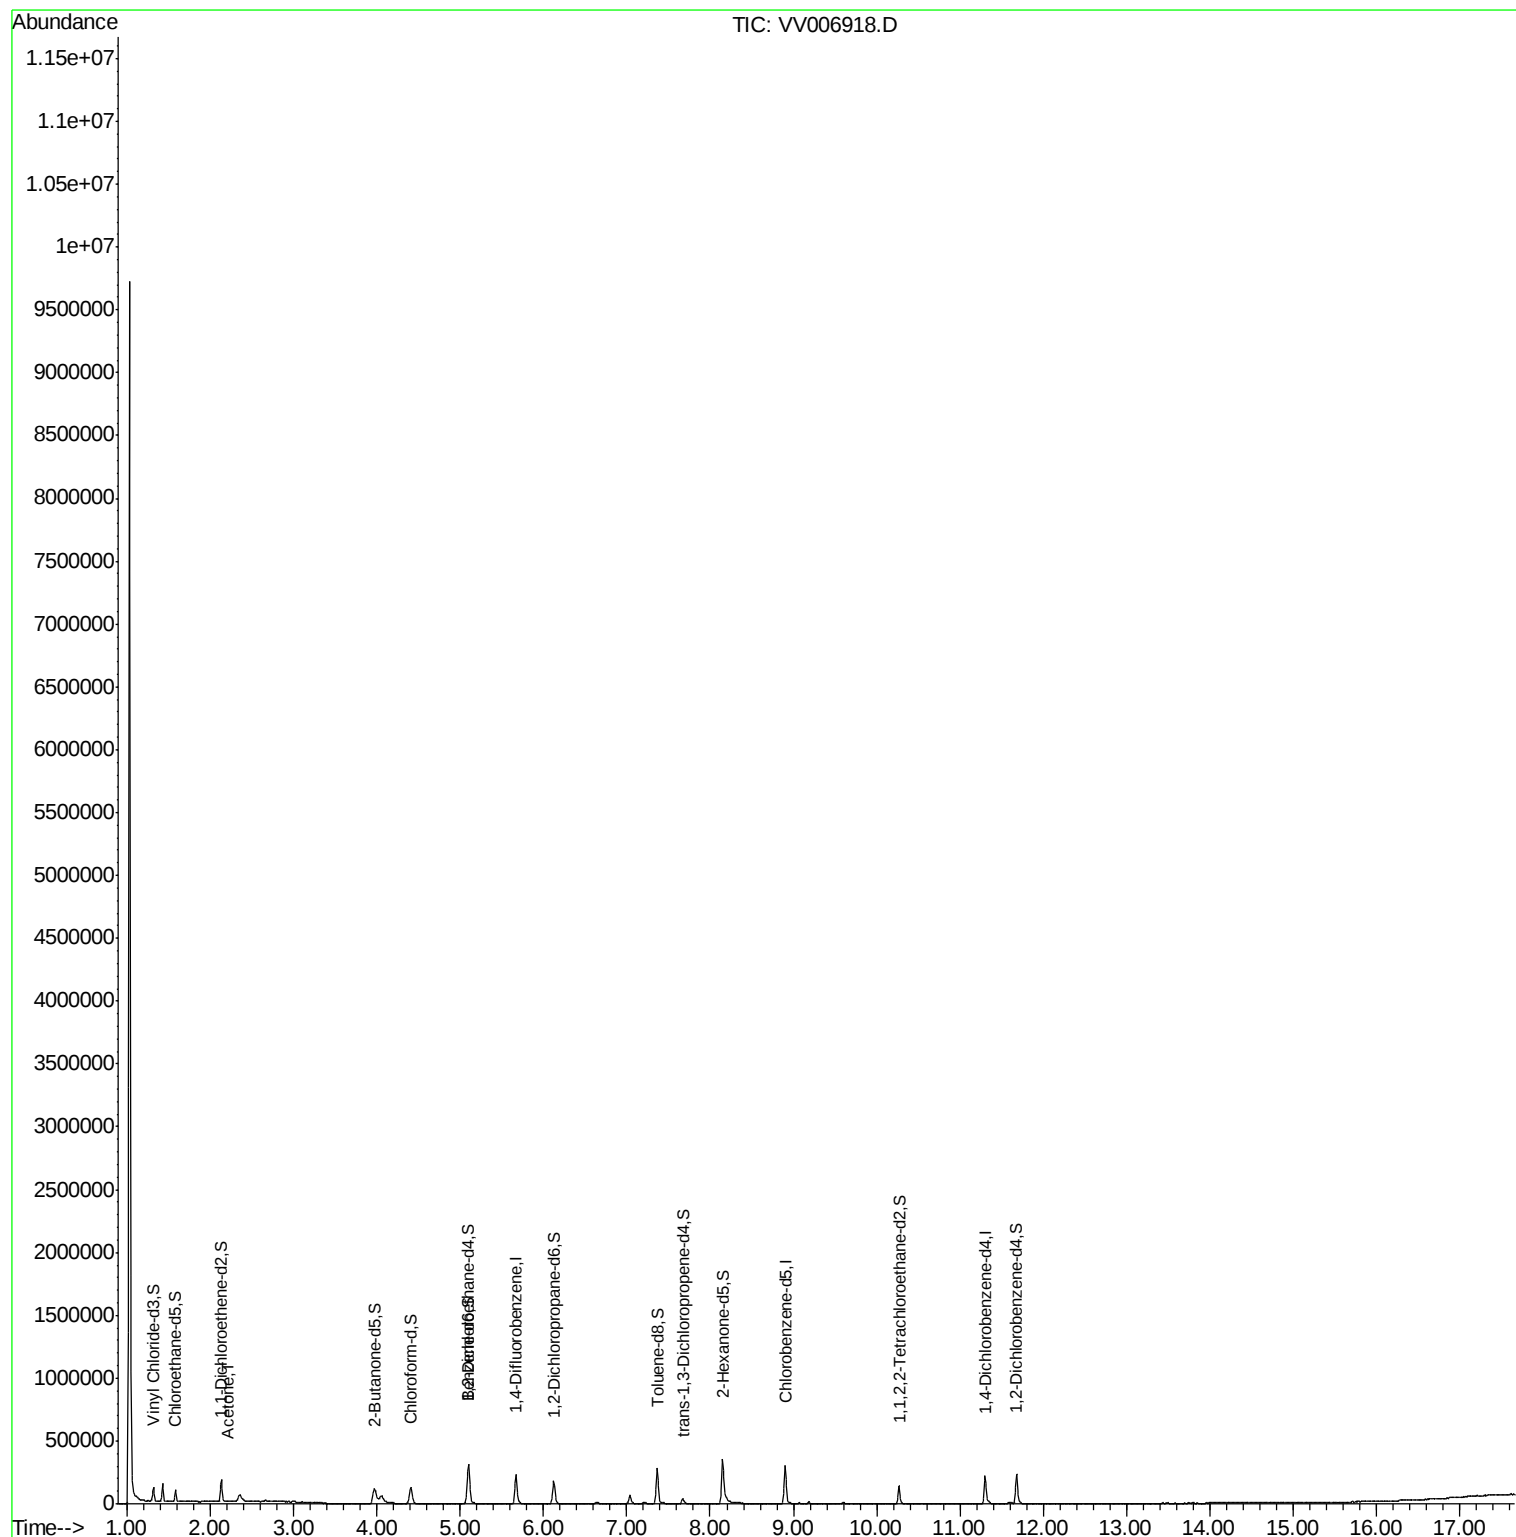

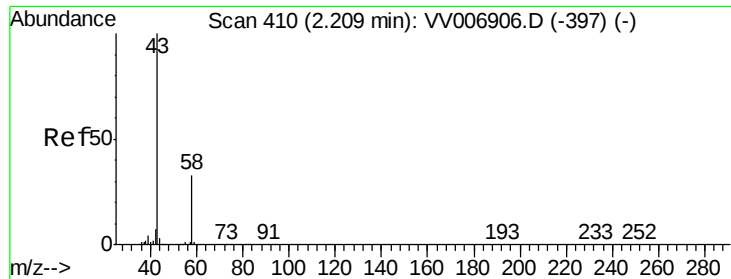

#13

Acetone

Concen: 3.97 ug/L

RT: 2.21 min Scan# 409

Delta R.T. -0.00 min

Lab File: VV006918.D

Acq: 08 Aug 2018 00:50

Instrument :
MSVOA_V
ClientSampleId :
ESWS6

Tot Ion: 43 Resp: 9223

Ion Ratio Lower Upper

43 100

58 39.0 0.0 68.0

