

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV080718\
 Data File : VV006922.D
 Acq On : 08 Aug 2018 02:37
 Operator : SY/MD
 Sample : J4357-14
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ESWT2

Quant Time: Aug 08 07:50:02 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080718WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Aug 08 07:06:57 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	187651	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	181183	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	67414	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	62313	5.54	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	110.80%
7) Chloroethane-d5	1.58	69	56863	5.17	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	103.40%
11) 1,1-Dichloroethene-d2	2.13	63	86058	3.72	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	74.40%
20) 2-Butanone-d5	3.97	46	208953	58.20	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	116.40%
24) Chloroform-d	4.41	84	125873	5.33	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.60%
26) 1,2-Dichloroethane-d4	5.09	65	70772	5.62	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	112.40%
32) Benzene-d6	5.10	84	236561	5.33	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.60%
36) 1,2-Dichloropropane-d6	6.12	67	84796	5.26	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	105.20%
41) Toluene-d8	7.37	98	170962	4.46	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.20%
43) trans-1,3-Dichloropropene-	7.67	79	22040	4.23	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.60%
46) 2-Hexanone-d5	8.15	63	103262	47.73	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	95.46%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	66172	5.47	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	109.40%
64) 1,2-Dichlorobenzene-d4	11.68	152	58052	5.32	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.40%


Target Compounds					Ovalue
13) Acetone	2.21	43	9139	3.90 ug/L	99
53) m,p-xylene	9.19	106	7134	0.38 ug/L	79


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV080718\
Data File : VV006922.D
Acq On : 08 Aug 2018 02:37
Operator : SY/MD
Sample : J4357-14
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ESWT2

Quant Time: Aug 08 07:50:02 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Aug 08 07:06:57 2018
Response via : Initial Calibration

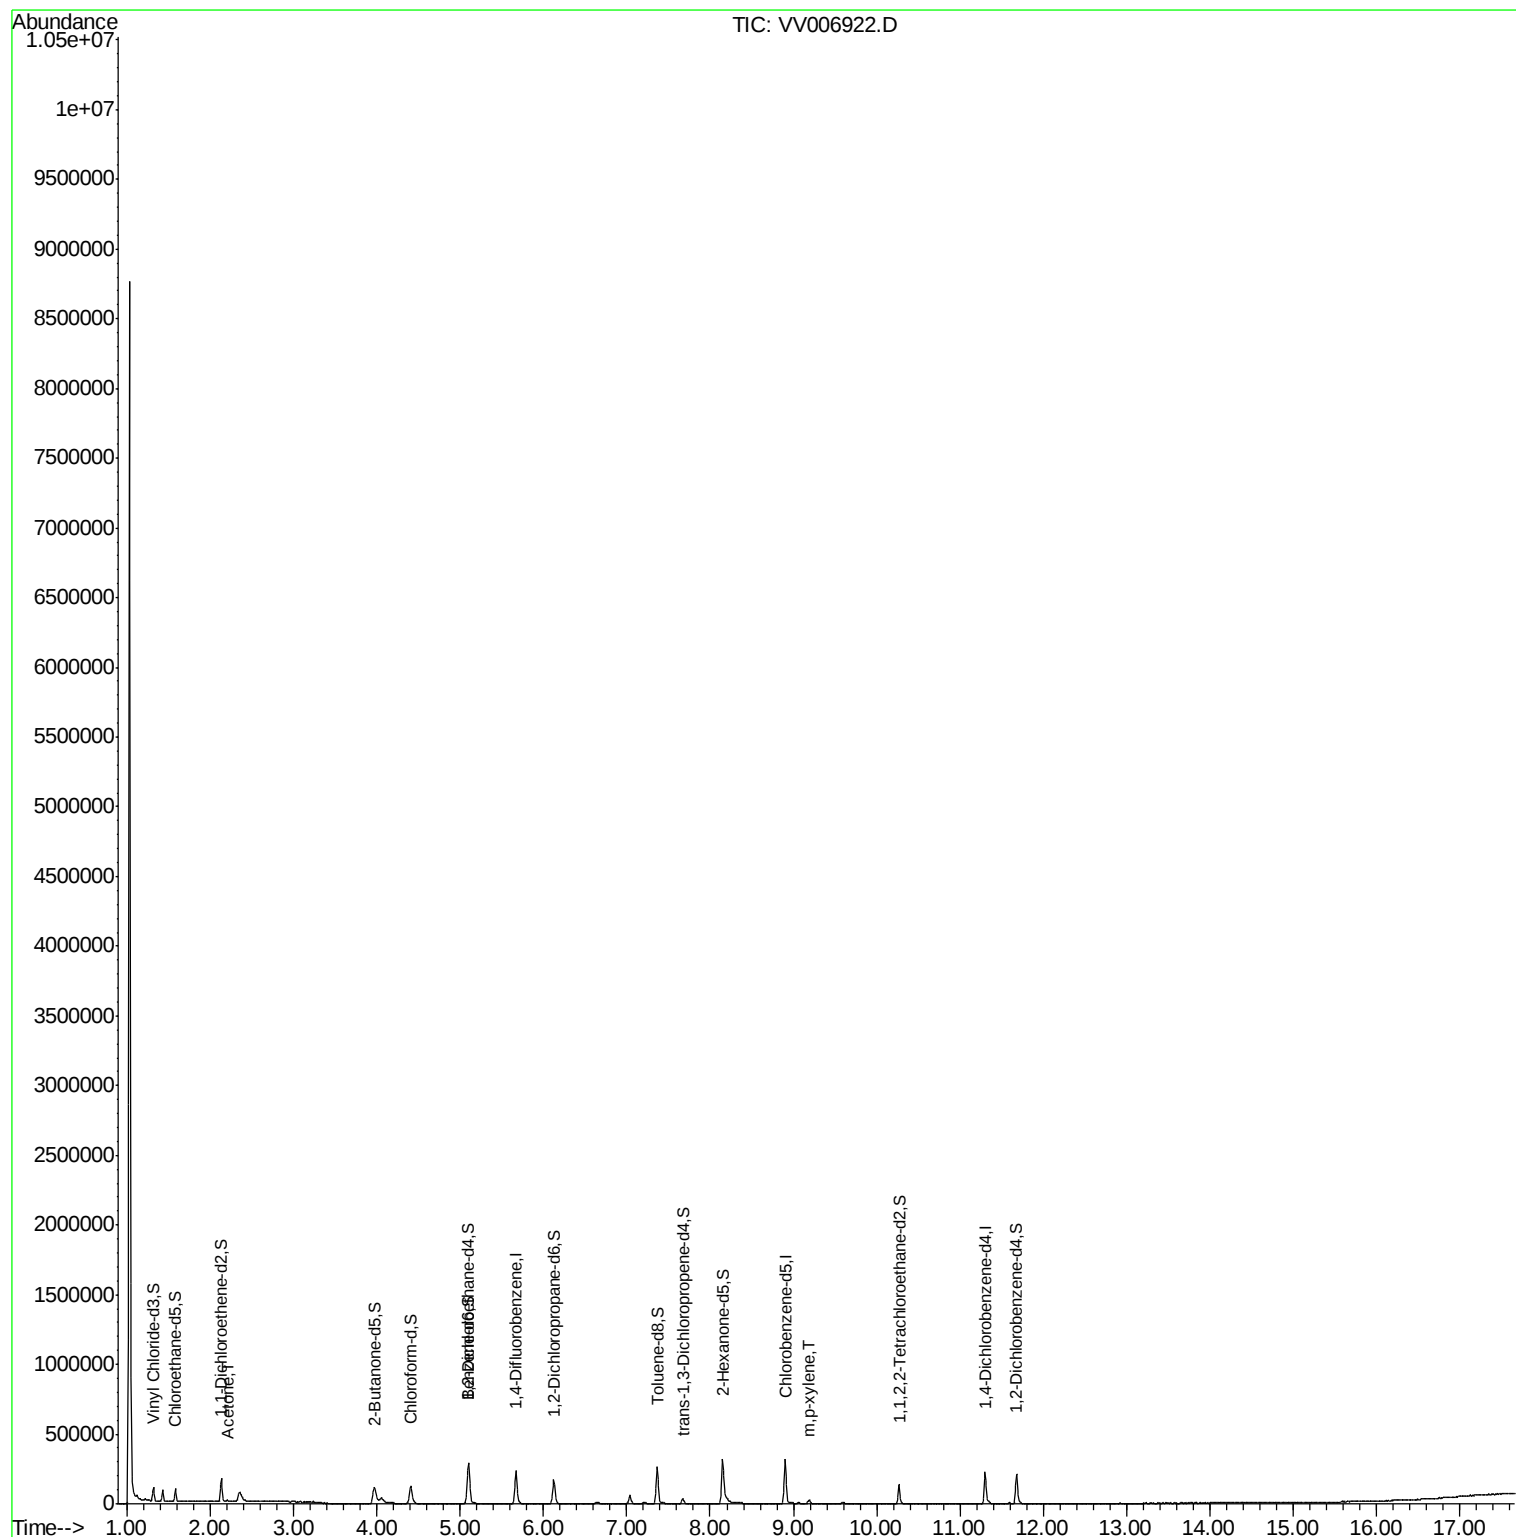

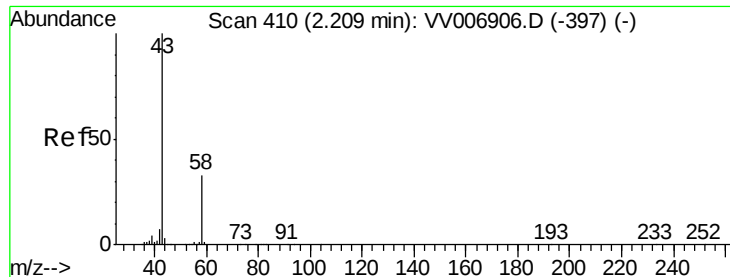

#13

Acetone

Concen: 3.90 ug/L

RT: 2.21 min Scan# 409

Delta R.T. -0.00 min

Lab File: VV006922.D

Acq: 08 Aug 2018 02:37

Instrument :

MSVOA_V

ClientSampleId :





ESWT2

Tot Ion: 43 Resp: 9139

Ion Ratio Lower Upper

43 100

58 33.6 0.0 68.0

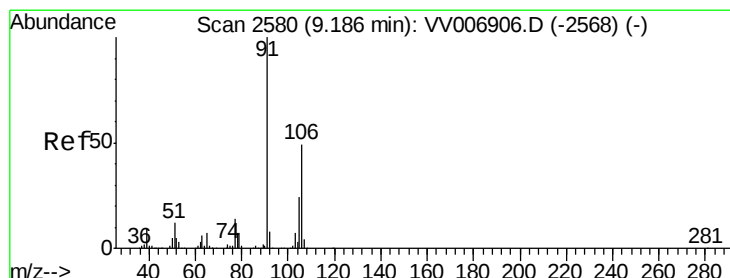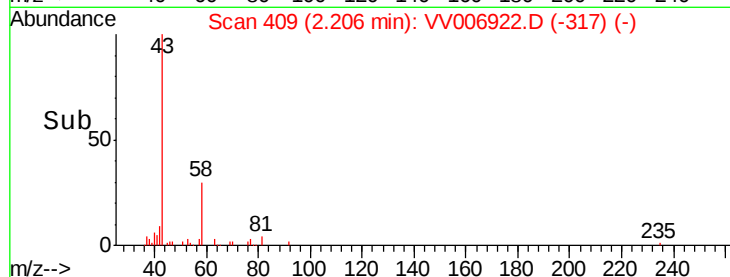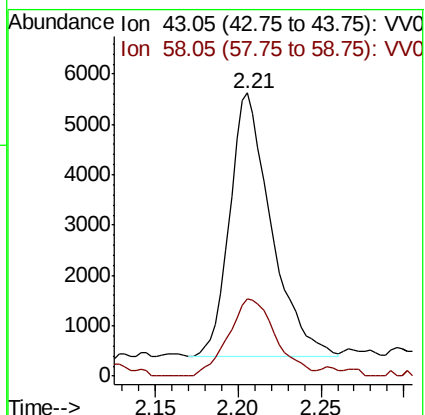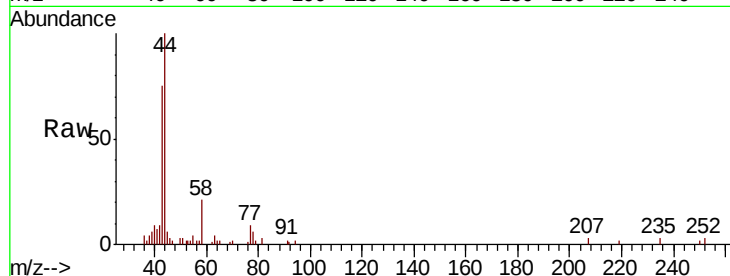

#53

m,p-xylene

Concen: 0.38 ug/L

RT: 9.19 min Scan# 2580

Delta R.T. 0.00 min

Lab File: VV006922.D

Acq: 08 Aug 2018 02:37

Tgt Ion: 106 Resp: 7134

Ion Ratio Lower Upper

106 100

91 178.4 147.7 274.3

