


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV080718\
 Data File : VV006899.D
 Acq On : 07 Aug 2018 15:44
 Operator : SY/MD
 Sample : BFB79
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB79

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080718WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Aug 08 07:06:57 2018

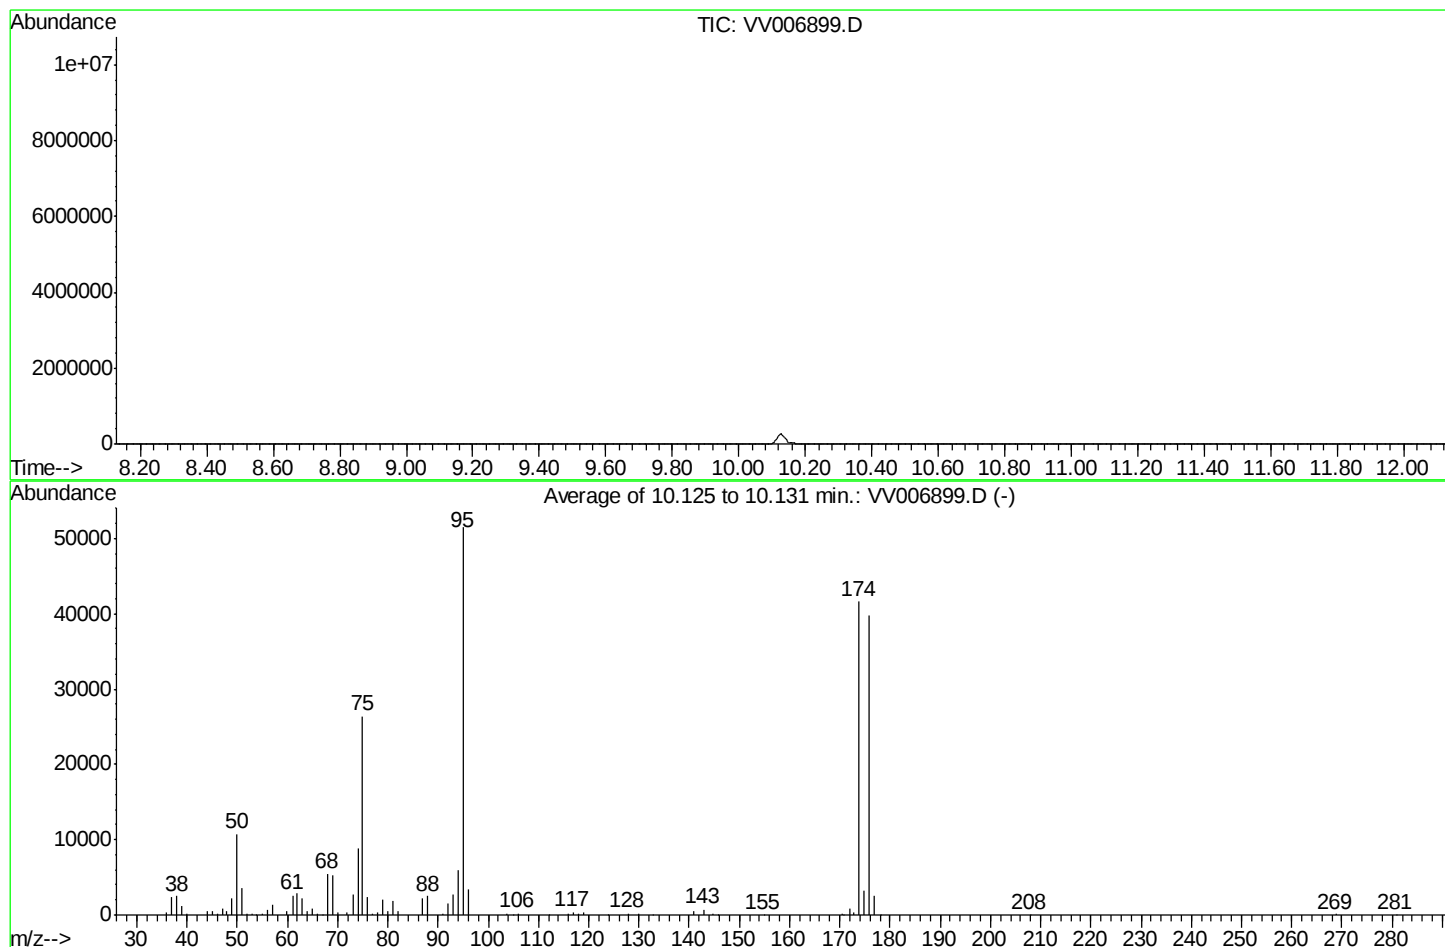

AutoFind: Scans 2872, 2873, 2874; Background Corrected with Scan 2858

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	10727	PASS
75	95	30	80	51.3	26432	PASS
95	95	100	100	100.0	51477	PASS
96	95	5	9	6.6	3420	PASS
173	174	0.00	2	1.0	414	PASS
174	95	50	120	80.8	41589	PASS
175	174	5	9	7.6	3170	PASS
176	174	95	101	95.7	39821	PASS
177	176	5	9	6.2	2488	PASS

Scan 2858 (10.080 min): VV006899.D
BFB79

m/z	Abundance
36.00	144.0
39.90	450.0
40.80	127.0
43.00	110.0
44.00	1402.0
45.10	115.0
68.80	138.0
76.80	121.0
207.00	289.0

Instrument :
MSVOA_V
ClientSampleId :
BFB79

m/z	Abundance
36.00	636.0
37.00	2370.0
38.00	2640.0
39.00	1385.0
39.90	622.0
40.90	104.0
43.00	126.0
44.00	1967.0
45.00	656.0
46.10	155.0
47.00	990.0
48.00	529.0
49.00	2252.0
50.00	11060.0
51.00	3707.0
52.00	239.0
52.90	178.0
54.90	210.0
56.00	891.0
57.00	1321.0
59.90	526.0
61.00	2725.0
62.00	3181.0
63.00	2275.0
64.00	534.0
64.90	870.0
65.80	197.0
67.00	214.0
68.00	5517.0
69.00	5601.0
70.00	490.0
71.90	295.0
73.00	2736.0
74.00	9137.0
75.00	27264.0
76.00	2303.0
76.90	346.0
78.10	257.0
78.90	2021.0
79.90	543.0
80.90	1970.0
82.00	454.0
86.90	2437.0
87.90	2443.0
90.90	217.0
91.90	1562.0
93.00	2892.0
94.00	6287.0
95.00	52768.0
96.00	3756.0
103.90	209.0
104.80	126.0
105.90	275.0
115.80	283.0
116.90	376.0
117.90	204.0
118.90	368.0
127.80	222.0
129.80	174.0
140.90	530.0
142.90	761.0
144.80	241.0
145.80	119.0
154.80	115.0
170.60	122.0
172.00	889.0
173.90	42144.0
174.90	3297.0
175.90	39896.0
176.90	2429.0
207.10	162.0
207.90	119.0
268.80	145.0

Instrument :
MSVOA_V
ClientSampleId :
BFB79

m/z	Abundance
35.90	510.0
37.00	2440.0
38.00	2576.0
39.00	1293.0
39.90	748.0
44.00	1941.0
44.90	704.0
46.10	140.0
47.00	882.0
48.00	495.0
49.00	2169.0
50.00	11103.0
51.00	3793.0
52.00	227.0
52.90	160.0
54.90	262.0
56.00	788.0
57.00	1443.0
60.00	535.0
61.00	2635.0
62.00	3019.0
63.00	2318.0
64.00	482.0
64.90	900.0
65.90	152.0
68.00	5636.0
69.00	5495.0
70.00	440.0
71.90	264.0
73.00	2912.0
74.00	9203.0
75.00	27184.0
76.00	2381.0
76.70	321.0
78.00	335.0
78.90	2167.0
80.00	518.0
80.90	1888.0
82.00	473.0
86.90	2306.0
87.90	2589.0
90.90	201.0
92.00	1611.0
93.00	2889.0
94.00	6129.0
95.00	53176.0
96.00	3522.0
103.80	143.0
104.90	102.0
106.00	267.0
115.80	249.0
116.80	457.0
117.90	226.0
118.90	339.0
127.80	210.0
129.80	190.0
140.90	566.0
143.00	733.0
144.90	255.0
154.80	108.0
170.60	168.0
172.10	874.0
172.80	666.0
173.90	42976.0
174.90	3234.0
175.90	41080.0
176.90	2524.0
178.00	121.0
207.00	172.0
208.00	123.0
268.80	147.0

Instrument :
MSVOA_V
ClientSampleId :
BFB79

m/z	Abundance
35.90	491.0
37.00	2287.0
38.00	2288.0
39.00	1146.0
39.90	739.0
43.00	115.0
44.00	1778.0
44.90	697.0
45.90	120.0
47.00	752.0
47.90	381.0
49.00	2092.0
50.00	10018.0
51.00	3402.0
52.00	228.0
53.00	139.0
53.80	105.0
54.90	277.0
55.90	607.0
56.90	1425.0
60.00	469.0
61.00	2457.0
62.00	2602.0
63.00	2183.0
64.00	417.0
64.90	799.0
68.00	5229.0
69.00	5016.0
70.00	313.0
72.00	234.0
73.00	2645.0
74.00	8279.0
75.00	24848.0
76.00	2352.0
76.80	282.0
78.00	307.0
78.90	1993.0
80.00	532.0
80.90	1758.0
81.90	450.0
86.90	1942.0
87.90	2387.0
90.80	184.0
92.00	1486.0
93.00	2469.0
94.00	5408.0
95.00	48488.0
96.00	2983.0
103.70	146.0
105.90	197.0
112.00	106.0
115.80	154.0
116.80	434.0
117.80	218.0
118.90	326.0
123.70	107.0
127.80	178.0
129.90	191.0
132.70	122.0
140.90	490.0
143.00	693.0
144.90	268.0
170.80	185.0
172.10	861.0
172.80	578.0
173.90	39648.0
174.90	2981.0
175.90	38488.0
176.90	2511.0
178.00	103.0
206.90	228.0
268.90	119.0
280.80	122.0

Instrument :
MSVOA_V
ClientSampleId :
BFB79