


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV080719\
 Data File : VV012119.D
 Acq On : 07 Aug 2019 11:11
 Operator : SY/MD
 Sample : BFB46
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB46

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM080619W.M
 Title : VOC Analysis
 Last Update : Thu Aug 08 13:16:01 2019

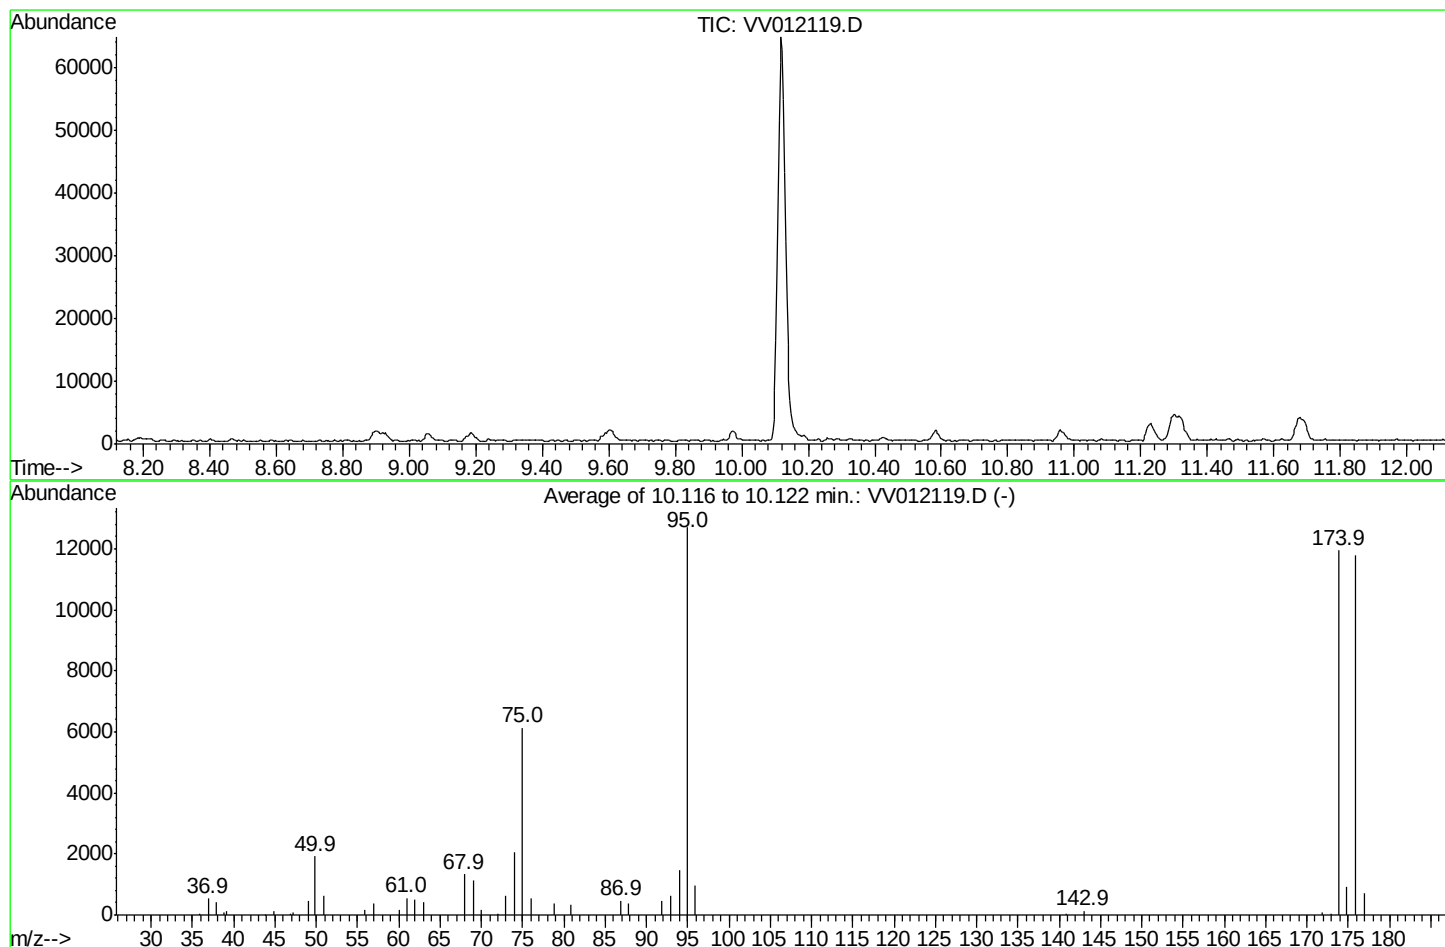

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.2	1928	PASS
75	95	30	80	48.3	6142	PASS
95	95	100	100	100.0	12705	PASS
96	95	5	9	7.5	952	PASS
173	174	0.00	2	0.5	56	PASS
174	95	50	120	94.0	11943	PASS
175	174	5	9	7.7	922	PASS
176	174	95	101	98.6	11773	PASS
177	176	5	9	6.1	715	PASS

m/z	Abundance
36.90	548.0
37.90	448.0
38.80	146.0
39.10	159.0
39.80	321.0
43.90	318.0
44.80	128.0
47.20	153.0
49.00	501.0
49.90	1992.0
51.00	659.0
56.00	182.0
56.90	387.0
60.00	152.0
61.00	582.0
62.00	537.0
63.00	435.0
67.90	1428.0
69.00	1121.0
70.00	193.0
72.90	668.0
73.90	2176.0
75.00	6266.0
76.00	516.0
78.80	379.0
80.90	365.0
86.90	495.0
87.80	396.0
91.90	489.0
92.90	654.0
94.00	1461.0
95.00	13029.0
95.90	994.0
143.00	154.0
171.80	132.0
173.90	12413.0
174.90	942.0
175.90	12255.0
176.90	735.0

Instrument :
MSVOA_V
ClientSampleId :
BFB46

m/z	Abundance
35.80	126.0
36.90	523.0
37.90	448.0
38.80	133.0
39.10	138.0
39.90	290.0
43.90	291.0
44.90	109.0
47.30	151.0
49.00	468.0
49.90	1775.0
51.00	560.0
56.00	173.0
56.90	340.0
60.00	191.0
60.90	556.0
62.00	560.0
62.90	441.0
67.90	1273.0
69.00	1011.0
70.00	184.0
72.00	114.0
72.90	737.0
73.90	2045.0
75.00	6218.0
76.00	547.0
78.80	326.0
80.90	340.0
86.90	455.0
87.70	351.0
91.90	450.0
92.90	593.0
94.00	1445.0
95.00	12284.0
96.00	956.0
140.90	116.0
142.90	164.0
171.90	130.0
172.90	169.0
173.90	11147.0
174.80	870.0
175.90	10828.0
176.90	733.0

Instrument :
MSVOA_V
ClientSampleId :
BFB46

Scan 2797 (10.084 min): VV012119.D
BFB46

m/z	Abundance
39.80	390.0
43.80	305.0

Instrument :
MSVOA_V
ClientSampleId :
BFB46

m/z	Abundance
36.90	532.0
37.90	384.0
39.10	149.0
39.80	329.0
43.90	340.0
44.80	128.0
46.90	124.0
49.00	449.0
49.90	2019.0
50.90	665.0
55.90	167.0
56.90	376.0
60.10	127.0
61.00	545.0
62.00	445.0
62.90	382.0
67.90	1317.0
69.00	1224.0
70.00	144.0
72.90	546.0
74.00	2003.0
75.00	5944.0
76.00	517.0
78.80	378.0
80.80	341.0
86.90	450.0
87.80	391.0
91.90	460.0
93.00	679.0
94.00	1441.0
95.00	12802.0
96.00	908.0
142.90	128.0
173.90	12271.0
174.90	954.0
175.90	12238.0
176.90	678.0

Instrument :
MSVOA_V
ClientSampleId :
BFB46