
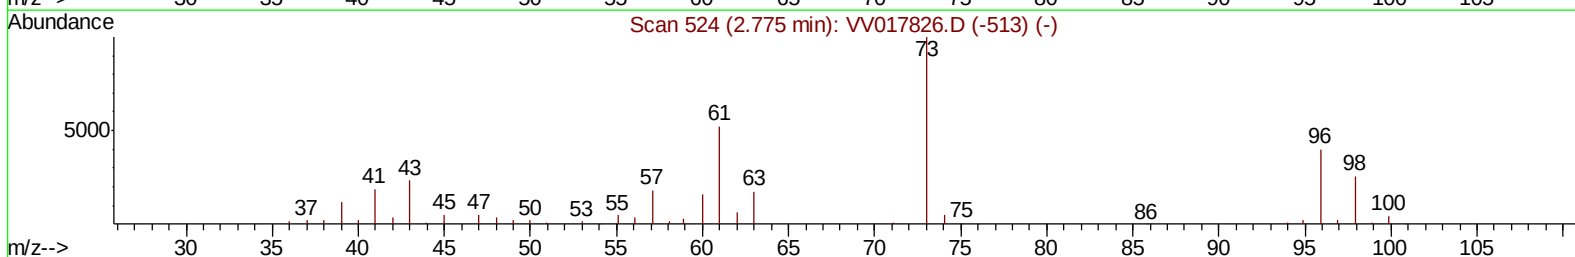
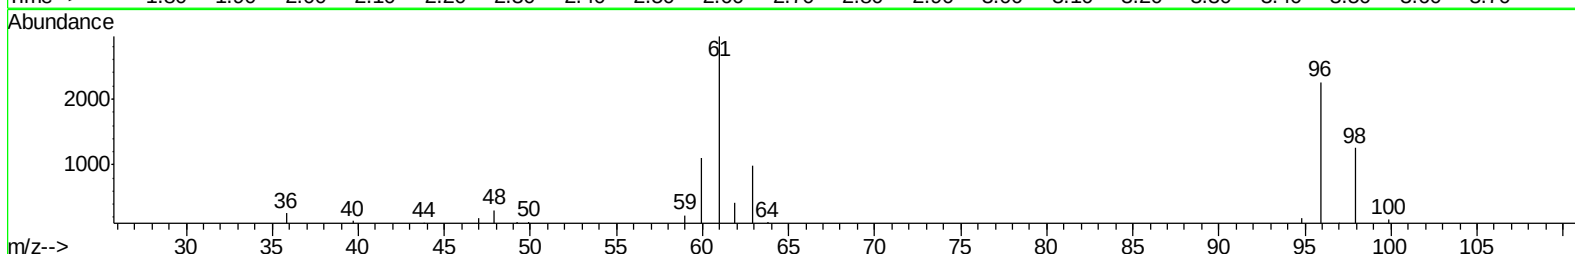


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV080720\
Data File : VV017836.D
Acq On : 07 Aug 2020 13:43
Operator : SY/MD
Sample : L3590-08
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Aug 08 00:25:27 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM073020WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Aug 08 00:22:47 2020
Response via : Initial Calibration

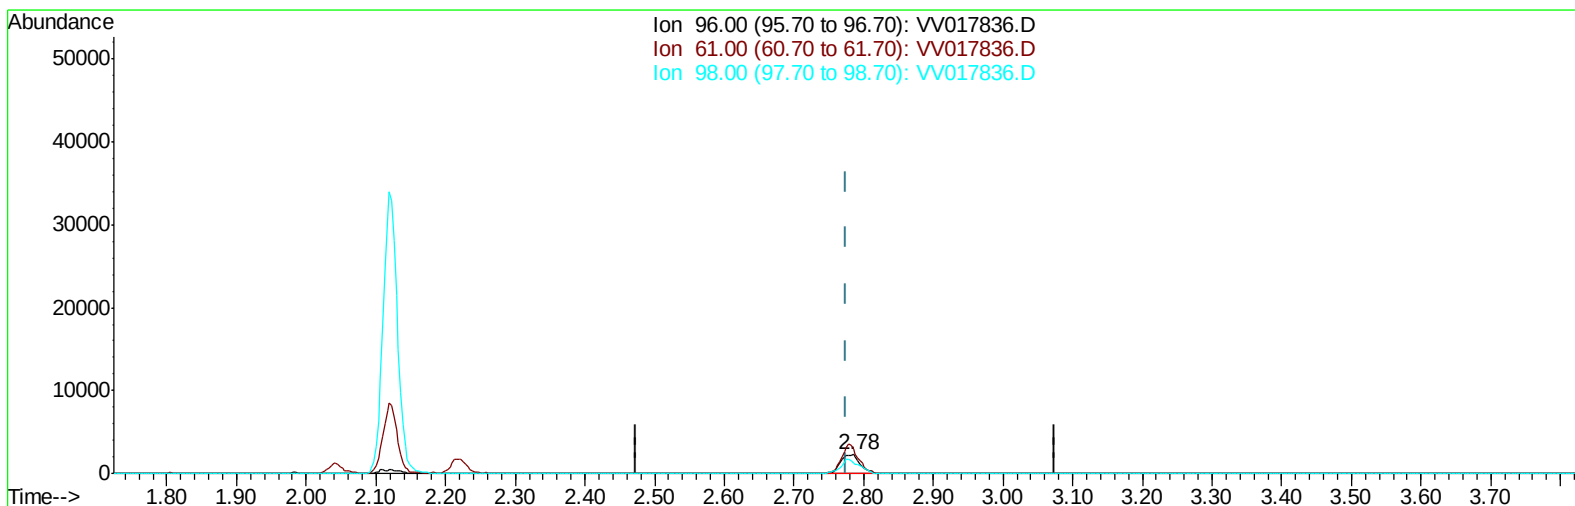

TIC: VV017836.D

(17) trans-1,2-Dichloroethene (T)

2.785min (+0.010) 3.00ug/L m

response 4393

Ion	Exp%	Act%
96.00	100	100
61.00	137.50	131.06
98.00	61.70	55.72
0.00	0.00	0.00