


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV080720\
Data File : VV017825.D
Acq On : 07 Aug 2020 09:05
Operator : SY/MD
Sample : BFB68
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB68

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM073020WMA.M
Title : VOC Analysis
Last Update : Sat Aug 08 03:52:38 2020

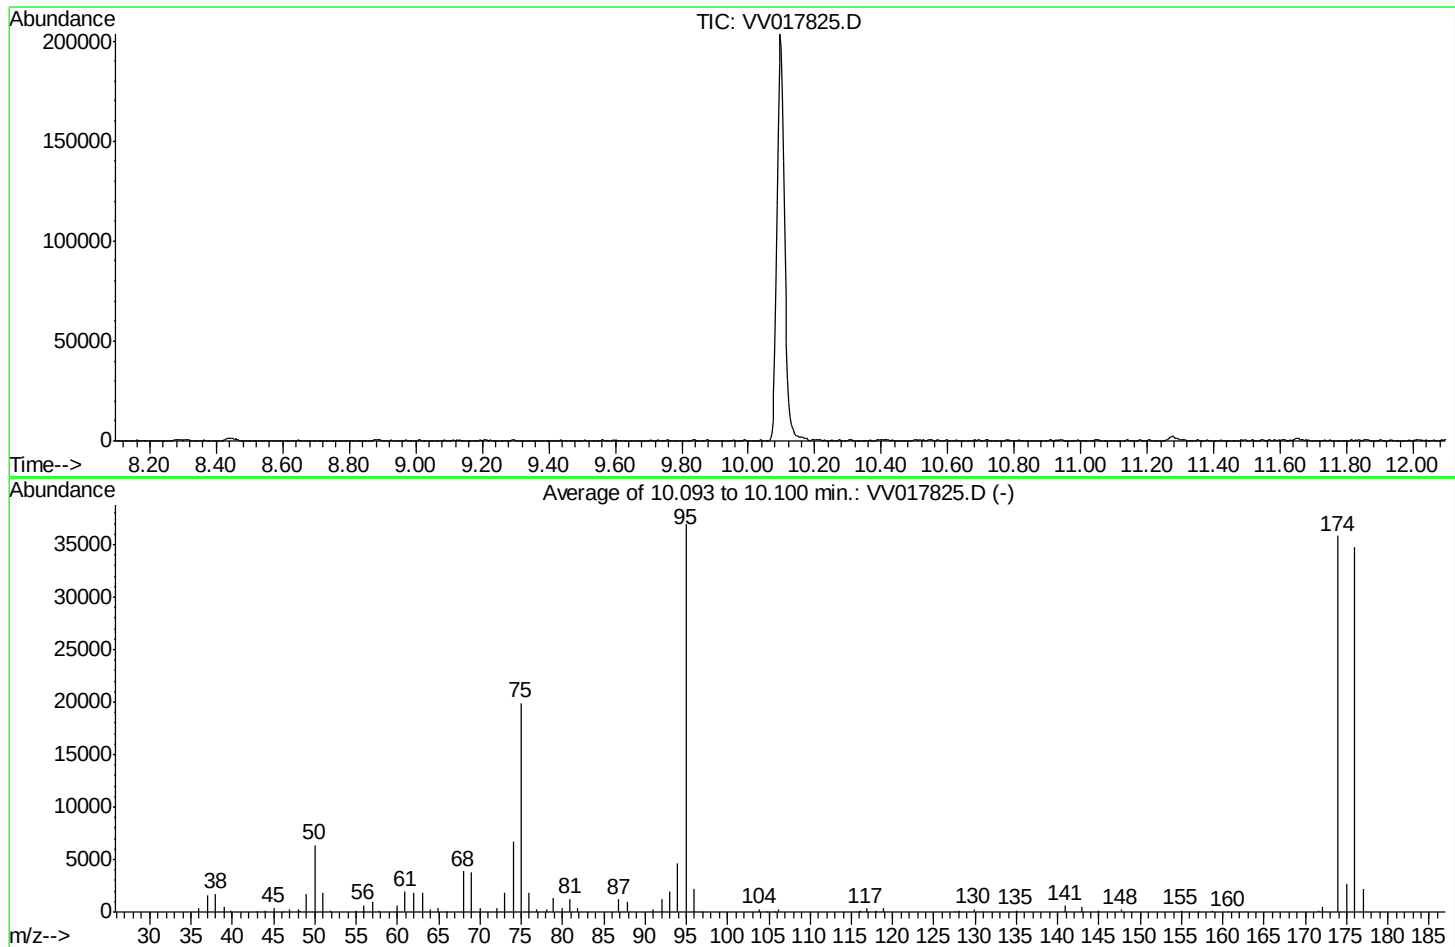

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2790

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	6347	PASS
75	95	30	80	53.9	19906	PASS
95	95	100	100	100.0	36933	PASS
96	95	5	9	6.1	2252	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	97.0	35813	PASS
175	174	5	9	7.4	2662	PASS
176	174	95	101	97.1	34781	PASS
177	176	5	9	6.2	2173	PASS

Scan 2790 (10.061 min): VV017825.D
BFB68

m/z	Abundance
43.90	168.0
147.30	111.0

Instrument :
MSVOA_V
ClientSampleId :
BFB68

m/z	Abundance
35.80	363.0
37.00	1541.0
38.00	1614.0
39.00	560.0
44.00	263.0
45.00	361.0
46.20	108.0
46.90	344.0
48.00	260.0
49.00	1706.0
50.00	6274.0
51.00	1750.0
51.90	130.0
55.10	138.0
55.90	597.0
56.90	1022.0
59.90	618.0
60.90	1908.0
62.00	1781.0
63.00	1761.0
64.00	290.0
64.90	362.0
66.00	107.0
68.00	3784.0
69.00	3565.0
70.00	392.0
72.00	395.0
73.00	1715.0
74.00	6522.0
75.00	19504.0
76.00	1873.0
76.90	255.0
78.00	207.0
78.80	1246.0
79.90	474.0
80.90	1345.0
81.90	308.0
86.80	1245.0
87.90	1011.0
90.90	249.0
92.00	1170.0
93.00	1974.0
94.00	4379.0
95.00	35360.0
96.00	1974.0
96.80	111.0
103.80	261.0
106.10	269.0
115.90	171.0
116.80	357.0
118.90	320.0
128.10	216.0
129.90	222.0
134.90	103.0
140.90	650.0
142.80	413.0
144.90	115.0
147.70	155.0
155.00	156.0
157.00	103.0
158.80	155.0
172.10	404.0
174.00	34008.0
175.00	2693.0
175.90	32784.0
176.90	2213.0

Instrument :
MSVOA_V
ClientSampleId :
BFB68

m/z	Abundance
35.90	447.0
37.00	1694.0
38.00	1765.0
39.00	504.0
39.90	134.0
44.10	247.0
45.00	380.0
47.00	285.0
48.00	270.0
48.20	274.0
49.00	1743.0
50.00	6580.0
51.00	1835.0
51.80	148.0
55.00	138.0
55.90	674.0
56.90	1111.0
57.80	113.0
59.90	748.0
60.90	1924.0
62.00	1823.0
63.00	1868.0
64.00	320.0
65.00	391.0
68.00	4002.0
69.00	3993.0
70.00	343.0
72.00	394.0
73.00	1932.0
74.00	6856.0
75.00	20600.0
76.00	1877.0
76.90	294.0
78.00	254.0
78.80	1338.0
79.90	454.0
80.90	1293.0
81.80	397.0
86.90	1247.0
87.90	1053.0
90.90	286.0
92.00	1276.0
93.00	2034.0
93.90	4776.0
95.00	38256.0
96.00	2323.0
103.90	290.0
106.10	223.0
116.10	166.0
116.80	379.0
118.00	122.0
118.80	305.0
128.10	191.0
129.90	244.0
134.90	125.0
140.90	619.0
142.80	521.0
144.90	171.0
147.70	201.0
155.00	175.0
158.70	109.0
160.60	102.0
171.60	242.0
172.10	486.0
173.90	37152.0
175.00	2717.0
175.90	36080.0
176.90	2222.0

Instrument :
MSVOA_V
ClientSampleId :
BFB68

m/z	Abundance
35.90	453.0
37.00	1674.0
38.00	1799.0
38.90	486.0
39.80	117.0
42.90	109.0
44.10	309.0
45.10	402.0
47.00	235.0
47.90	250.0
49.00	1527.0
50.00	6187.0
51.00	1770.0
51.80	129.0
55.00	159.0
55.90	613.0
57.00	970.0
57.80	108.0
59.90	659.0
61.00	1882.0
62.00	1820.0
63.00	1748.0
64.00	276.0
65.00	337.0
68.00	3874.0
69.00	3917.0
70.00	332.0
72.00	321.0
73.10	1796.0
74.00	6760.0
75.00	19616.0
76.00	1753.0
76.90	258.0
78.10	275.0
78.90	1353.0
79.90	366.0
80.90	1208.0
81.80	444.0
86.90	1096.0
87.90	989.0
90.90	275.0
92.00	1295.0
93.00	1834.0
93.90	4751.0
95.00	37184.0
96.00	2461.0
103.90	310.0
104.80	122.0
105.70	124.0
106.00	131.0
116.20	134.0
116.80	306.0
117.90	142.0
118.70	311.0
127.60	135.0
128.10	104.0
129.80	276.0
130.90	113.0
135.00	177.0
140.90	522.0
142.90	617.0
145.00	202.0
147.70	210.0
154.90	180.0
171.50	250.0
172.10	465.0
173.90	36280.0
175.00	2577.0
175.90	35480.0
177.00	2084.0

Instrument :
MSVOA_V
ClientSampleId :
BFB68