


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV080818\
 Data File : VV006929.D
 Acq On : 08 Aug 2018 08:54
 Operator : SY/MD
 Sample : BFB80
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB80

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080718WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Aug 09 07:05:51 2018

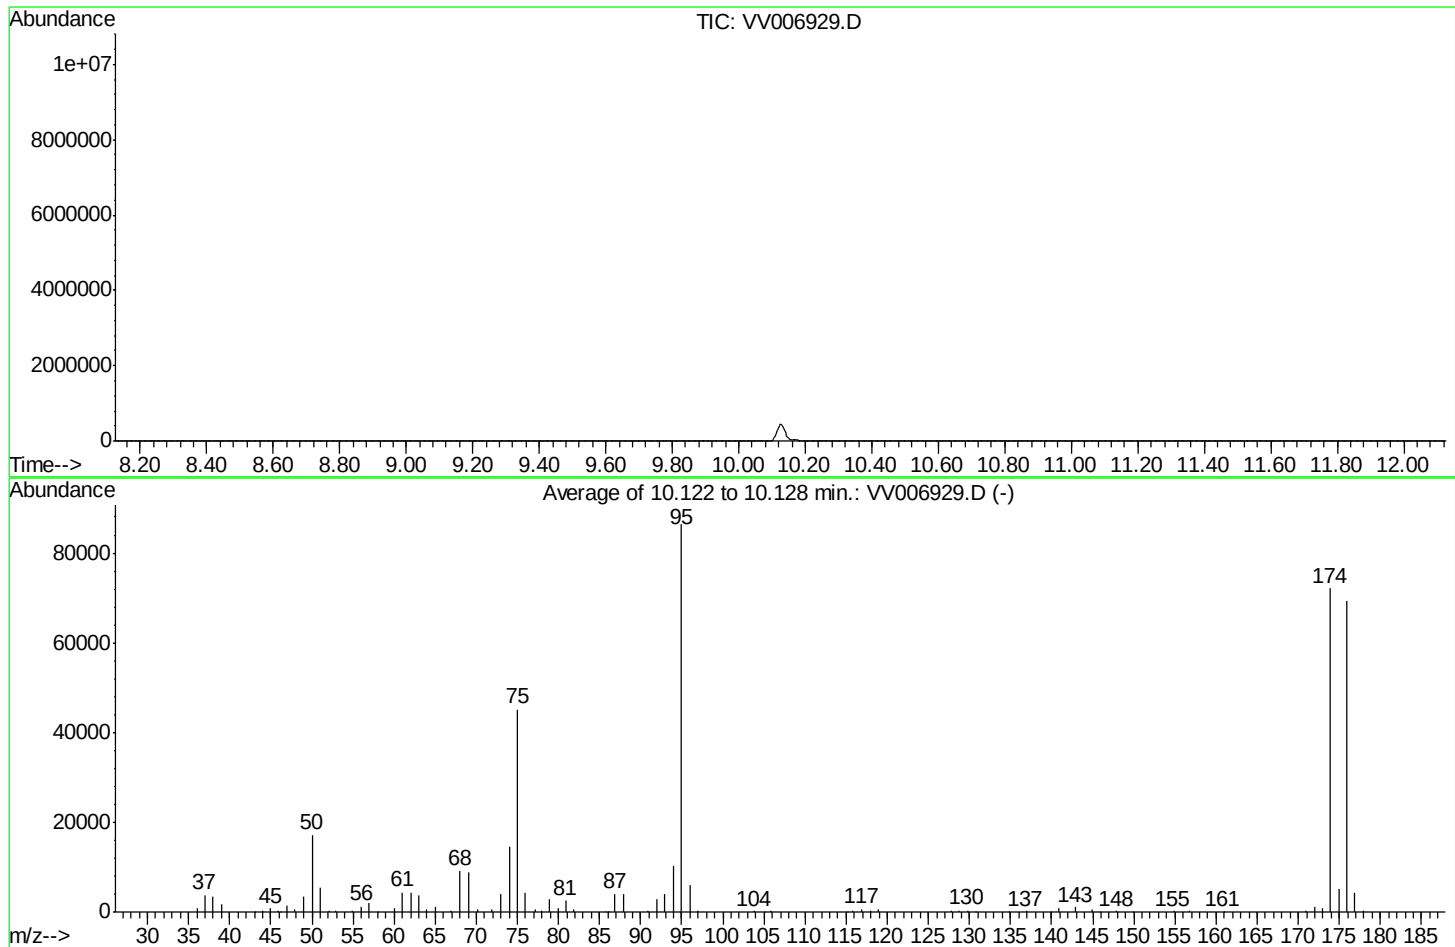

AutoFind: Scans 2871, 2872, 2873; Background Corrected with Scan 2858

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	17122	PASS
75	95	30	80	52.3	45173	PASS
95	95	100	100	100.0	86381	PASS
96	95	5	9	7.1	6137	PASS
173	174	0.00	2	1.1	769	PASS
174	95	50	120	83.4	72029	PASS
175	174	5	9	7.3	5261	PASS
176	174	95	101	96.3	69349	PASS
177	176	5	9	6.2	4271	PASS

Scan 2858 (10.080 min): VV006929.D
BFB80

m/z	Abundance
40.00	567.0
44.00	1274.0
77.90	132.0
207.10	273.0

Instrument :
MSVOA_V
ClientSampleId :
BFB80

m/z	Abundance
36.10	757.0
37.00	3513.0
38.00	3369.0
39.00	1825.0
39.90	435.0
43.00	149.0
44.00	1673.0
45.00	694.0
45.90	290.0
46.90	1537.0
48.00	459.0
49.00	3281.0
50.00	16920.0
51.00	5360.0
52.10	310.0
52.90	186.0
54.90	210.0
56.00	1225.0
57.00	2021.0
58.00	129.0
60.00	832.0
61.00	4221.0
62.00	3902.0
63.00	3547.0
64.00	583.0
65.00	1200.0
66.90	265.0
68.00	8929.0
69.00	8528.0
70.10	474.0
71.90	508.0
73.00	3942.0
74.00	13897.0
75.00	43584.0
76.00	3925.0
77.10	688.0
78.10	484.0
78.90	2874.0
79.90	843.0
80.90	2365.0
81.90	703.0
85.80	154.0
86.90	3931.0
87.90	3837.0
90.80	362.0
92.00	2753.0
93.00	3683.0
94.00	9724.0
95.00	81776.0
96.00	6121.0
96.90	202.0
103.90	294.0
105.00	123.0
105.80	248.0
115.20	106.0
115.90	239.0
116.90	597.0
118.00	236.0
118.90	540.0
127.70	248.0
128.70	137.0
129.80	254.0
134.80	132.0
136.90	158.0
139.90	117.0
140.90	879.0
142.90	999.0
144.90	501.0
145.90	128.0
147.80	127.0
149.90	101.0
155.00	254.0
156.80	170.0
170.90	170.0
172.00	1051.0
172.90	731.0
173.90	67144.0
174.90	5034.0
175.90	63944.0
176.90	4250.0
177.90	137.0
207.00	205.0

Instrument :
MSVOA_V
ClientSampleId :
BFB80

m/z	Abundance
36.10	853.0
37.00	3850.0
38.00	3650.0
39.00	1749.0
39.90	550.0
43.10	156.0
44.00	1739.0
45.00	787.0
45.90	238.0
46.90	1579.0
47.90	471.0
49.00	3557.0
50.00	17696.0
51.00	5763.0
52.00	283.0
52.80	191.0
54.80	192.0
56.00	1265.0
57.00	2095.0
58.00	127.0
60.00	970.0
61.00	4491.0
62.00	4408.0
63.00	4001.0
64.00	679.0
65.00	1215.0
66.80	230.0
68.00	9552.0
69.00	9105.0
70.10	574.0
71.90	562.0
73.00	4273.0
74.00	14903.0
75.00	46648.0
76.00	4364.0
77.10	681.0
78.00	397.0
78.90	2922.0
79.90	884.0
80.90	2538.0
81.90	726.0
86.00	172.0
86.90	4247.0
87.90	4172.0
90.90	326.0
92.00	2839.0
93.00	4009.0
94.00	10664.0
95.00	89136.0
96.00	6339.0
96.90	251.0
103.90	281.0
105.00	142.0
105.80	269.0
115.90	315.0
116.90	641.0
118.00	336.0
118.90	565.0
127.80	287.0
128.70	181.0
129.80	301.0
134.80	126.0
137.00	179.0
139.90	108.0
140.90	928.0
142.90	1074.0
144.90	556.0
145.90	148.0
147.90	161.0
154.80	246.0
156.80	171.0
170.90	163.0
172.00	1117.0
172.90	799.0
173.90	74120.0
174.90	5413.0
175.90	71736.0
176.90	4340.0
177.90	207.0
207.00	180.0

Instrument :
MSVOA_V
ClientSampleId :
BFB80

m/z	Abundance
36.10	821.0
37.00	4025.0
38.00	3607.0
39.00	1598.0
39.90	584.0
43.10	124.0
44.00	1682.0
45.00	812.0
45.80	153.0
46.20	157.0
47.00	1372.0
47.90	479.0
49.00	3715.0
50.00	16752.0
51.00	5546.0
52.00	280.0
52.80	160.0
54.90	174.0
56.00	1200.0
57.00	2012.0
60.00	1047.0
61.00	4348.0
62.00	4478.0
63.00	3967.0
64.00	793.0
65.00	1091.0
66.80	184.0
68.00	9128.0
69.00	8971.0
70.10	651.0
71.90	552.0
73.00	4093.0
74.00	14888.0
75.00	45288.0
76.00	4445.0
77.10	717.0
78.00	266.0
78.90	2866.0
79.90	934.0
80.90	2706.0
81.90	691.0
86.00	220.0
86.90	4161.0
87.90	4010.0
91.00	293.0
92.00	2661.0
92.90	3987.0
94.00	10622.0
95.00	88232.0
96.00	5952.0
97.00	244.0
103.80	274.0
105.00	118.0
105.80	245.0
115.80	367.0
116.90	637.0
118.00	374.0
118.80	558.0
127.90	325.0
128.70	148.0
129.80	393.0
130.70	103.0
134.80	126.0
137.00	155.0
140.80	926.0
142.90	1095.0
144.90	552.0
145.90	144.0
148.00	210.0
154.70	229.0
156.80	166.0
160.90	145.0
170.90	167.0
171.90	1174.0
172.90	778.0
173.90	74824.0
174.90	5337.0
175.90	72368.0
176.90	4223.0
177.90	196.0
207.00	172.0

Instrument :
MSVOA_V
ClientSampleId :
BFB80