

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV080819\
 Data File : VV012141.D
 Acq On : 08 Aug 2019 23:30
 Operator : SY/MD
 Sample : K4184-05
 Misc : 25mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA2

Quant Time: Aug 09 07:08:57 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080819WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Aug 09 06:44:52 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	105435	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	98433	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	54701	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	23271	5.19	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	103.80%
7) Chloroethane-d5	1.58	69	16474	5.00	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	100.00%
11) 1,1-Dichloroethene-d2	2.13	63	34316	3.78	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	75.60%
20) 2-Butanone-d5	3.94	46	15347	13.25	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	26.50%#
24) Chloroform-d	4.40	84	59258	4.55	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.00%
26) 1,2-Dichloroethane-d4	5.08	65	35932	5.30	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.00%
32) Benzene-d6	5.10	84	121771	5.03	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.60%
36) 1,2-Dichloropropane-d6	6.12	67	32189	5.04	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.80%
41) Toluene-d8	7.36	98	120393	4.91	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.20%
43) trans-1,3-Dichloropropene-	7.66	79	15046	4.51	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.20%
46) 2-Hexanone-d5	8.13	63	44401	41.82	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	83.64%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	26163	4.97	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.40%
64) 1,2-Dichlorobenzene-d4	11.67	152	52884	5.20	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.00%


Target Compounds					Ovalue
13) Acetone	2.19	43	2806	4.118 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV080819\
Data File : VV012141.D
Acq On : 08 Aug 2019 23:30
Operator : SY/MD
Sample : K4184-05
Misc : 25mL/MSVOA V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA2

Quant Time: Aug 09 07:08:57 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080819WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Aug 09 06:44:52 2019
Response via : Initial Calibration

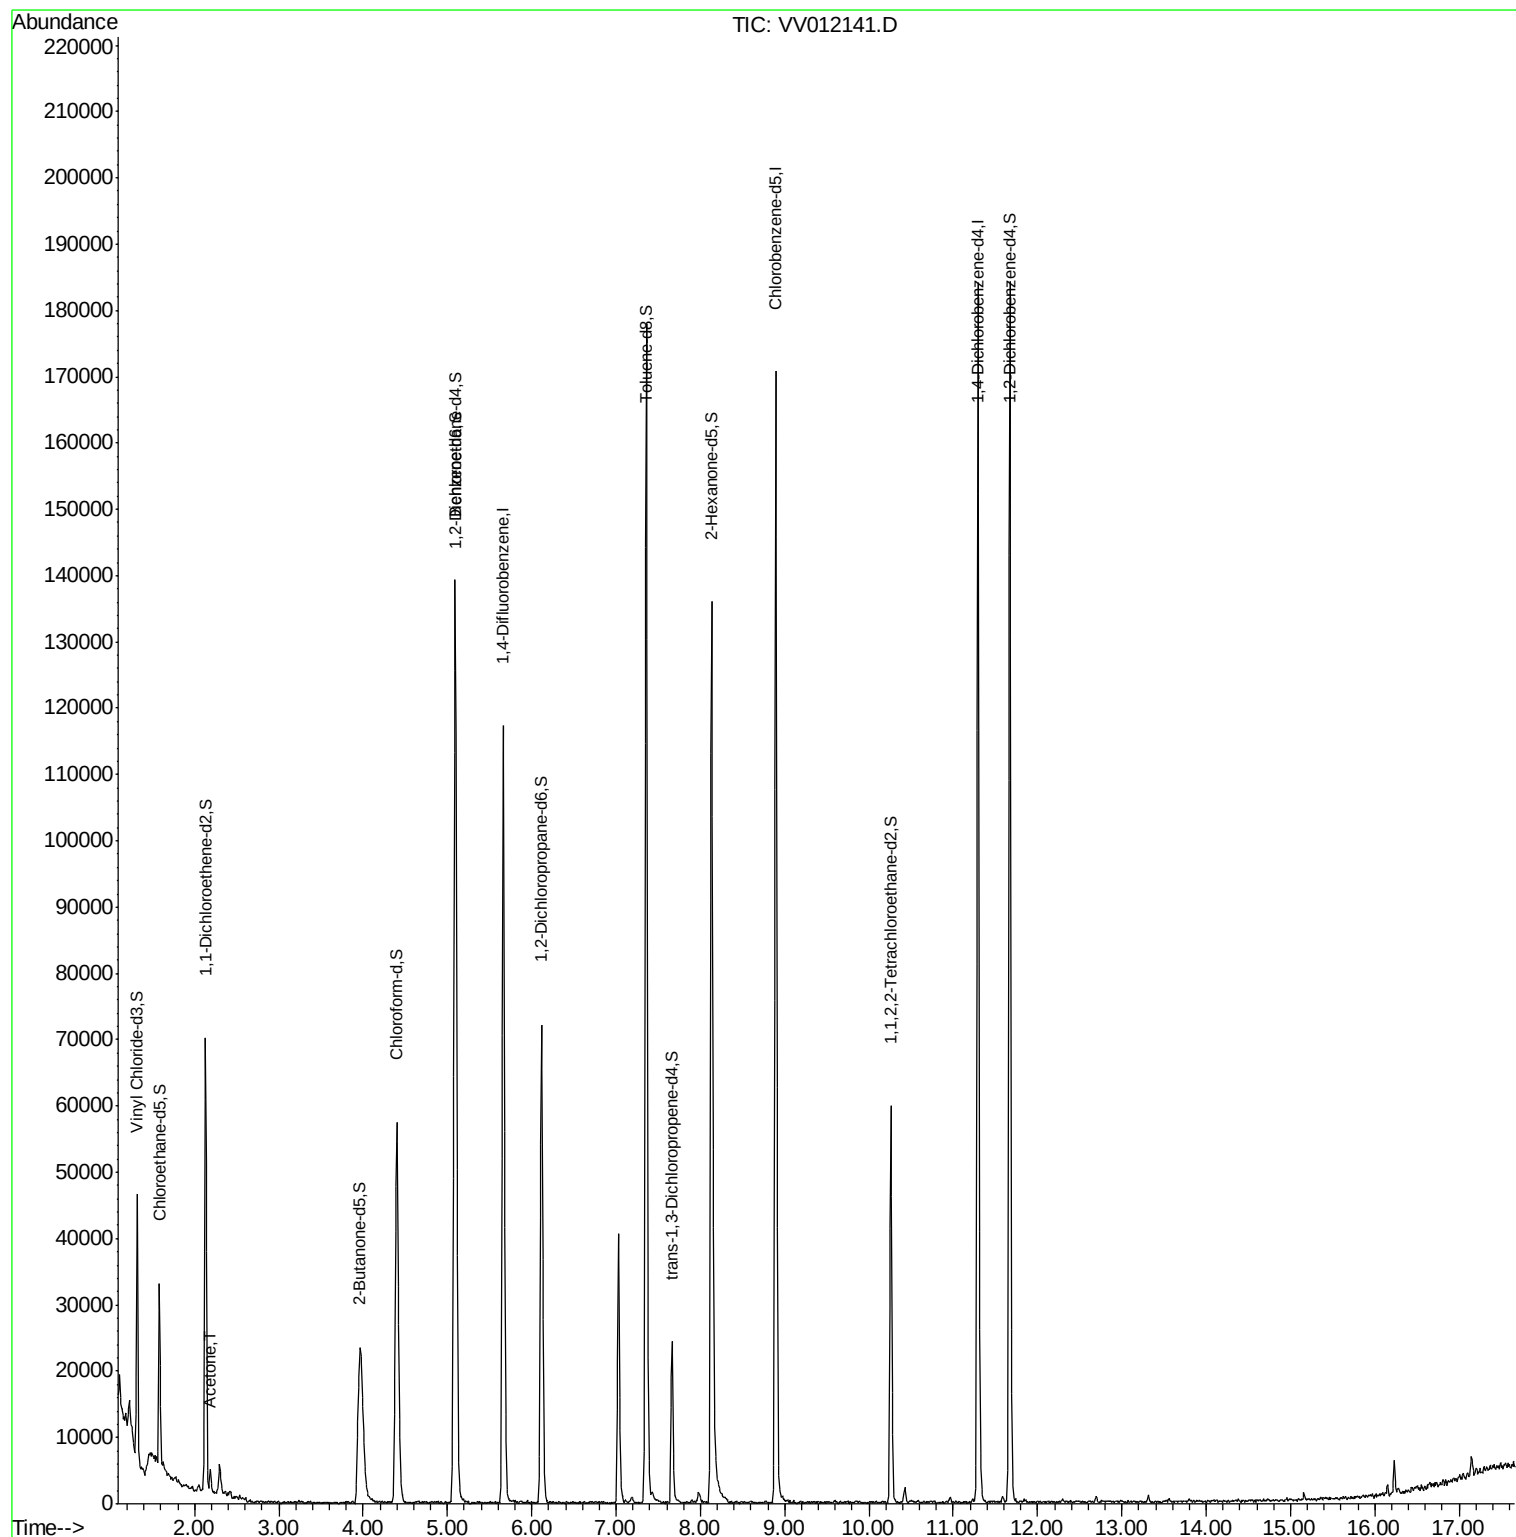

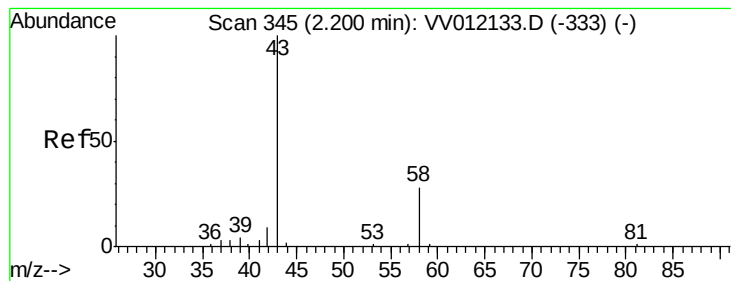

#13
 Acetone
 Concen: 4.118 ug/L
 RT: 2.19 min Scan# 341
 Delta R.T. -0.01 min
 Lab File: VV012141.D
 Acq: 08 Aug 2019 23:30

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA2

Tot Ion: 43 Resp: 2806
 Ion Ratio Lower Upper
 43 100
 58 26.8 0.0 54.6

