


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV080819\
 Data File : VV012130.D
 Acq On : 08 Aug 2019 16:33
 Operator : SY/MD
 Sample : BFB44
 Misc : 25mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB44

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080819WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Aug 09 17:51:52 2019

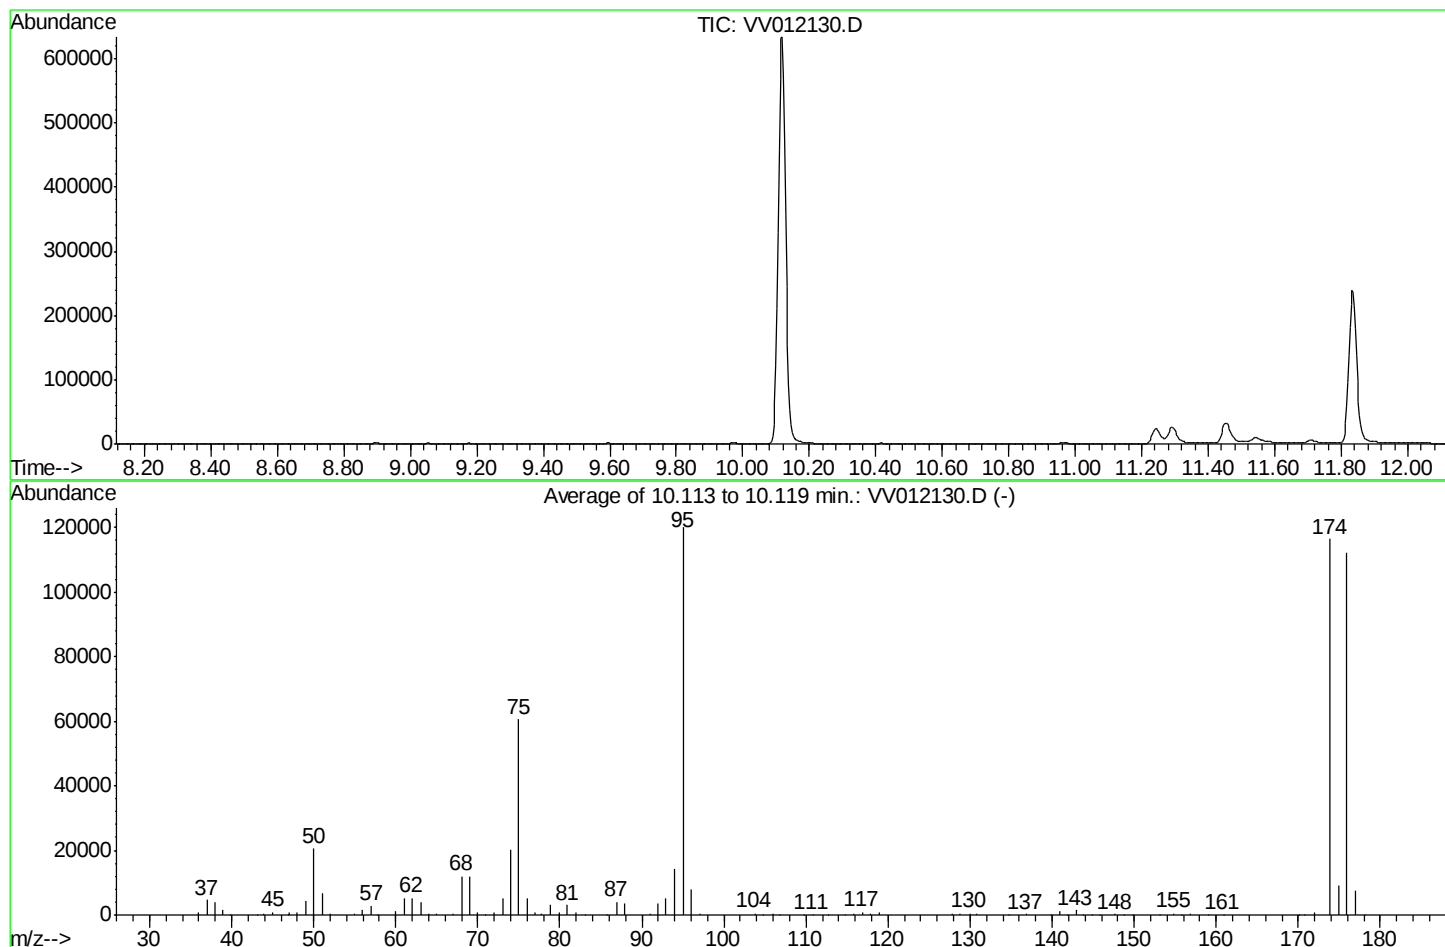

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	20450	PASS
75	95	30	80	50.5	60578	PASS
95	95	100	100	100.0	120072	PASS
96	95	5	9	6.8	8116	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	97.0	116450	PASS
175	174	5	9	8.0	9313	PASS
176	174	95	101	96.3	112096	PASS
177	176	5	9	6.8	7622	PASS

m/z	Abundance
36.00	977.0
36.90	4371.0
37.90	3826.0
38.90	1577.0
39.90	152.0
43.10	124.0
43.90	647.0
45.00	869.0
46.90	629.0
47.00	628.0
47.90	669.0
49.00	4247.0
50.00	19320.0
51.00	6594.0
51.90	322.0
54.90	308.0
56.00	1417.0
57.00	2851.0
57.90	178.0
60.00	1002.0
61.00	5006.0
61.90	5150.0
63.00	3528.0
64.00	493.0
64.90	300.0
67.00	293.0
68.00	10936.0
69.00	11196.0
70.00	819.0
72.00	612.0
73.00	4723.0
74.00	18992.0
75.00	57080.0
76.00	5069.0
77.00	637.0
77.80	365.0
78.90	2868.0
79.80	802.0
80.90	2837.0
81.90	713.0
86.90	3830.0
87.90	3442.0
91.00	525.0
91.90	3480.0
93.00	4859.0
93.90	13553.0
95.00	113208.0
96.00	7646.0
97.10	262.0
103.80	448.0
104.70	112.0
105.90	439.0
106.80	120.0
110.80	127.0
112.70	112.0
114.80	106.0
115.90	432.0
116.90	835.0
117.80	356.0
118.90	591.0
127.80	429.0
128.80	270.0
129.90	404.0
130.90	231.0
134.80	154.0
136.90	292.0
139.90	115.0
140.90	1173.0
141.90	211.0
142.90	1499.0
143.80	107.0
144.90	182.0
145.70	175.0
147.70	322.0
148.80	116.0
149.80	179.0
153.10	111.0
154.90	470.0
156.80	240.0
159.00	109.0
160.90	153.0
170.70	134.0
171.90	546.0
173.90	105368.0
174.90	8583.0
175.90	101312.0
176.90	7156.0
178.00	238.0

Instrument :
MSVOA_V
ClientSampleId :
BFB44

m/z	Abundance
36.00	1006.0
37.00	4870.0
38.00	4046.0
39.00	1715.0
39.90	178.0
43.10	128.0
43.90	691.0
45.00	1030.0
47.00	835.0
47.90	749.0
49.00	4600.0
50.00	21240.0
51.00	6852.0
52.00	293.0
55.00	399.0
56.00	1440.0
57.00	3092.0
57.90	156.0
60.00	1127.0
61.00	5345.0
62.00	5406.0
63.00	3903.0
64.00	554.0
65.00	313.0
66.90	284.0
68.00	12481.0
69.00	12174.0
70.00	793.0
70.80	126.0
72.00	696.0
73.00	5120.0
74.00	21064.0
75.00	62560.0
76.00	5291.0
77.00	690.0
77.80	404.0
78.90	3106.0
79.80	879.0
80.90	3073.0
81.90	772.0
83.10	123.0
86.90	4182.0
87.90	3781.0
91.00	507.0
92.00	3737.0
93.00	5364.0
94.00	15012.0
95.00	124144.0
96.00	8483.0
97.00	262.0
103.80	484.0
104.80	120.0
106.00	512.0
106.80	140.0
109.80	128.0
110.80	127.0
112.80	122.0
114.80	142.0
115.90	432.0
116.90	929.0
117.90	360.0
118.90	700.0
127.80	413.0
128.80	328.0
130.00	459.0
130.80	243.0
134.80	154.0
136.90	317.0
139.90	155.0
140.90	1317.0
141.90	214.0
142.90	1558.0
144.90	166.0
145.80	205.0
147.70	371.0
148.80	102.0
149.80	157.0
153.10	131.0
154.90	473.0
156.80	250.0
159.00	101.0
160.90	158.0
170.10	112.0
170.80	148.0
172.00	639.0
173.90	120232.0
174.90	9636.0
175.90	115592.0
177.00	7900.0
178.00	213.0

Instrument :
MSVOA_V
ClientSampleId :
BFB44

m/z	Abundance
35.90	910.0
37.00	4833.0
38.00	4077.0
39.00	1653.0
39.90	213.0
43.00	116.0
43.90	685.0
45.00	950.0
47.00	919.0
48.00	684.0
49.00	4579.0
50.00	20792.0
51.00	6364.0
52.00	239.0
55.00	449.0
55.90	1468.0
57.00	3008.0
57.80	138.0
60.00	1162.0
61.00	5183.0
62.00	5212.0
63.00	4105.0
63.90	529.0
65.00	340.0
66.90	256.0
68.00	12433.0
69.00	11901.0
69.90	765.0
70.80	120.0
72.00	747.0
73.00	5136.0
74.00	20888.0
75.00	62096.0
76.00	5245.0
77.00	728.0
77.80	412.0
78.90	3049.0
79.90	980.0
80.90	3070.0
81.90	755.0
83.10	121.0
85.70	131.0
87.00	4109.0
87.90	3703.0
90.90	445.0
92.00	3729.0
92.90	5364.0
94.00	14852.0
95.00	122864.0
96.00	8219.0
97.00	238.0
103.80	520.0
104.90	142.0
105.90	501.0
106.80	133.0
109.80	110.0
110.80	115.0
114.70	142.0
115.80	385.0
116.90	917.0
117.90	411.0
118.90	728.0
127.80	346.0
128.80	310.0
129.90	426.0
130.90	209.0
134.70	145.0
136.80	296.0
139.90	176.0
140.90	1331.0
141.80	201.0
142.90	1456.0
144.90	124.0
145.90	230.0
147.70	364.0
149.90	163.0
153.00	109.0
154.80	392.0
155.70	155.0
156.80	224.0
158.80	125.0
160.90	151.0
170.10	121.0
170.80	150.0
172.00	649.0
173.90	123752.0
174.90	9722.0
175.90	119384.0
176.90	7812.0
178.10	182.0

Instrument :
MSVOA_V
ClientSampleId :
BFB44

Scan 2794 (10.074 min): VV012130.D
BFB44

m/z	Abundance
39.80	149.0
44.10	216.0

Instrument :
MSVOA_V
ClientSampleId :
BFB44