

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV080820\
 Data File : VV017867.D
 Acq On : 08 Aug 2020 20:32
 Operator : SY/MD
 Sample : L3608-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F2L47

Manual Integrations
 APPROVED

MMDadoda
 8/10/2020 1:35:24 PM

Quant Time: Aug 10 06:10:27 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM080820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Aug 10 05:09:16 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	235944	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	220021	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	112367	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	34995	28.72	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	57.44%#
7) Chloroethane-d5	1.58	69	38386	37.08	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	74.16%
11) 1,1-Dichloroethene-d2	2.12	63	79865	27.28	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	54.56%#
21) 2-Butanone-d5	3.91	46	81679	107.05	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	107.05%
24) Chloroform-d	4.38	84	140567	44.00	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.00%
26) 1,2-Dichloroethane-d4	5.06	65	111159	47.89	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.78%
32) Benzene-d6	5.07	84	235272	46.31	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.62%
36) 1,2-Dichloropropane-d6	6.09	67	65035	50.48	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	100.96%
41) Toluene-d8	7.34	98	237769	46.56	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	93.12%
43) trans-1,3-Dichloropropene-	7.64	79	33254	40.09	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	80.18%
47) 2-Hexanone-d5	8.11	63	56238	120.53	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	120.53%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	98401	49.00	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	98.00%
64) 1,2-Dichlorobenzene-d4	11.65	152	118652	51.80	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	103.60%

Target Compounds

					Ovalue
5) Vinyl chloride	1.32	62	4452	3.229 ug/L #	80
17) trans-1,2-Dichloroethene	2.78	96	1150m	0.811 ug/L	
20) cis-1,2-Dichloroethene	3.94	96	169015	110.302 ug/L	99
34) Trichloroethene	5.94	95	1489m	0.947 ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV080820\
Data File : VV017867.D
Acq On : 08 Aug 2020 20:32
Operator : SY/MD
Sample : L3608-01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 27 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
F2L47

Manual Integrations
APPROVED

MMDadoda
8/10/2020 1:35:24 PM

Quant Time: Aug 10 06:10:27 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM080820WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Aug 10 05:09:16 2020
Response via : Initial Calibration

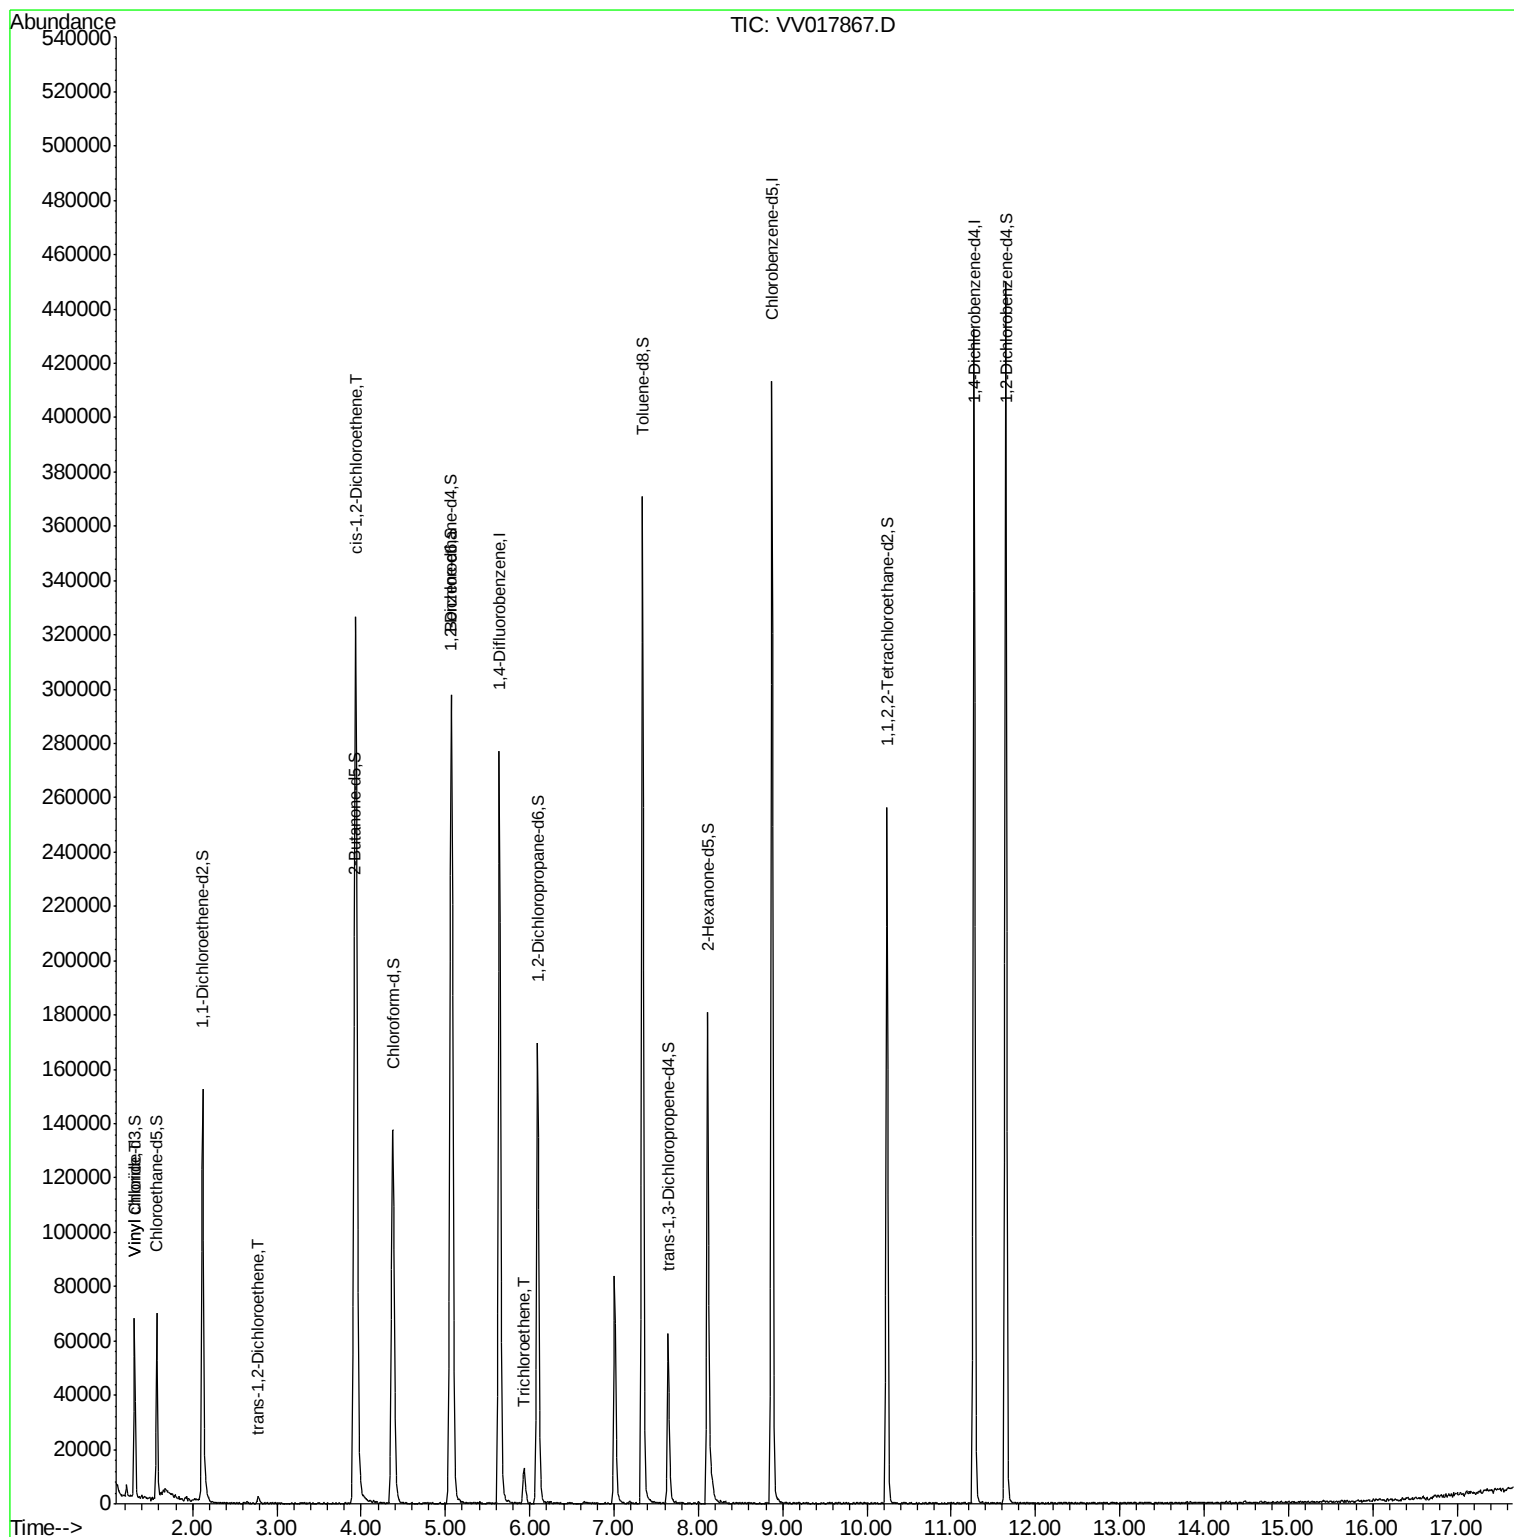

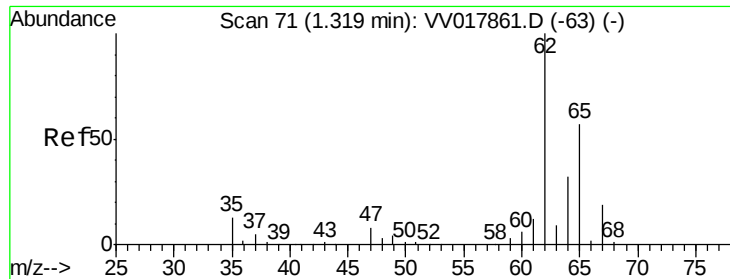

#5

Vinyl chloride

Concen: 3.229 ug/L

RT: 1.32 min Scan# 71

Delta R.T. -0.00 min

Lab File: VV017867.D

Acq: 08 Aug 2020 20:32

Instrument :

MSVOA_V

ClientSampled :

F2L47

Tot Ion: 62 Resp: 4452

Ion Ratio Lower Upper

62 100


64 45.8 24.0 44.6#

Manual Integrations

APPROVED




MMDadoda

8/10/2020 1:35:24 PM

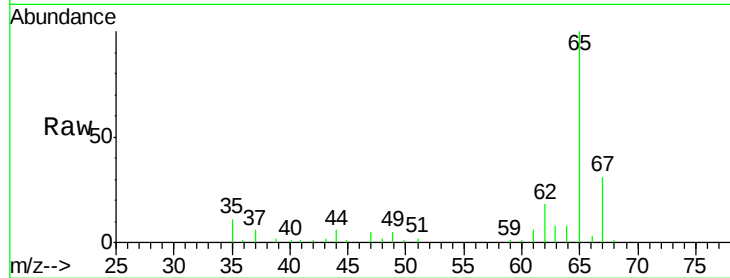

Abundance Ion 62.00 (61.70 to 62.70): VV0

Ion 64.00 (63.70 to 64.70): VV0

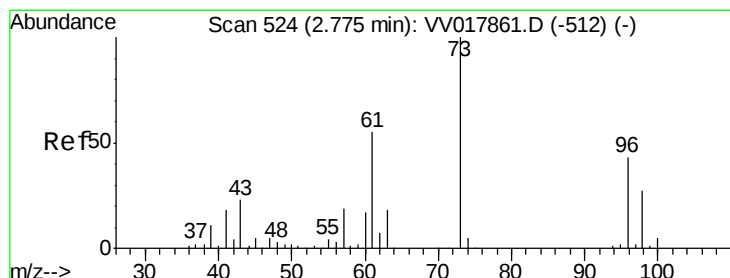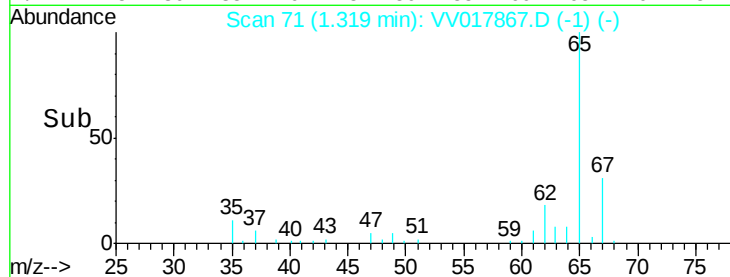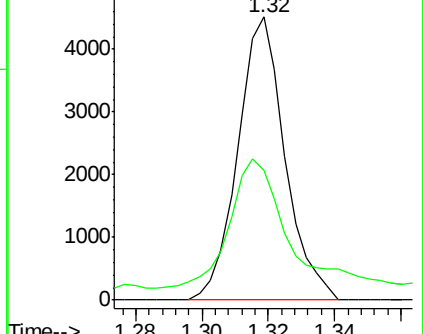

#17

trans-1,2-Dichloroethene

Concen: 0.811 ug/L m

RT: 2.78 min Scan# 526

Delta R.T. 0.01 min

Lab File: VV017867.D

Acq: 08 Aug 2020 20:32


Tgt Ion: 96 Resp: 1150

Ion Ratio Lower Upper

96 100

61 117.5 92.4 171.6



98 55.0 47.5 88.1

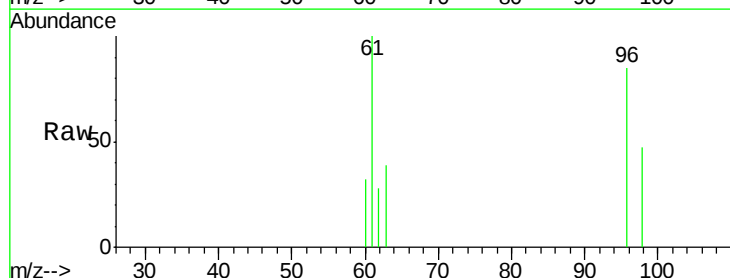


Abundance Ion 96.00 (95.70 to 96.70): VV0

Ion 61.00 (60.70 to 61.70): VV0

Ion 98.00 (97.70 to 98.70): VV0

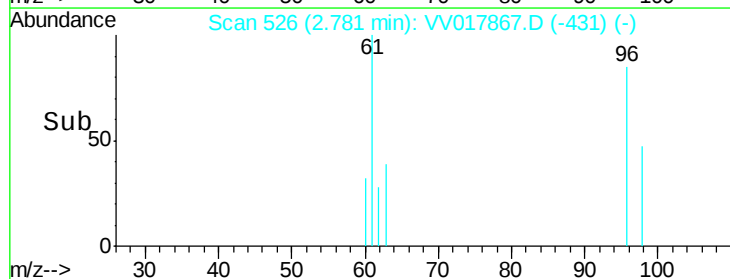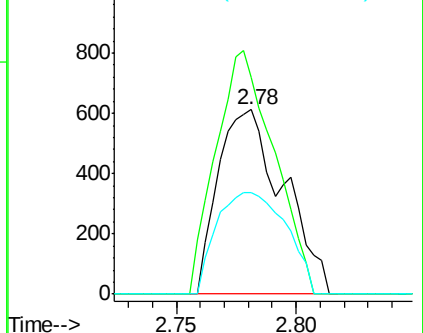

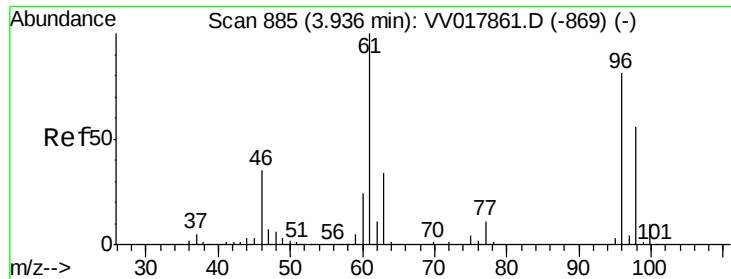





#20
cis-1,2-Dichloroethene
Concen: 110.302 ug/L
RT: 3.94 min Scan# 885
Delta R.T. -0.00 min
Lab File: VV017867.D
Acq: 08 Aug 2020 20:32

Instrument :
MSVOA_V
ClientSampleId :
F2L47

Tot Ion	Ion	Ratio	Resp	Lower	Upper
96	100		169015		
61	121.7	84.4	156.8		
68	0.0	0.0	0.0		

Manual Integrations
APPROVED

MMDadoda
8/10/2020 1:35:24 PM

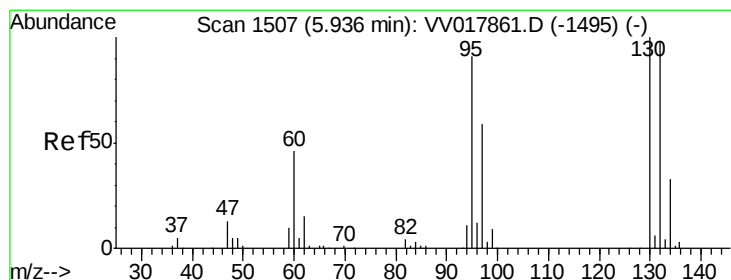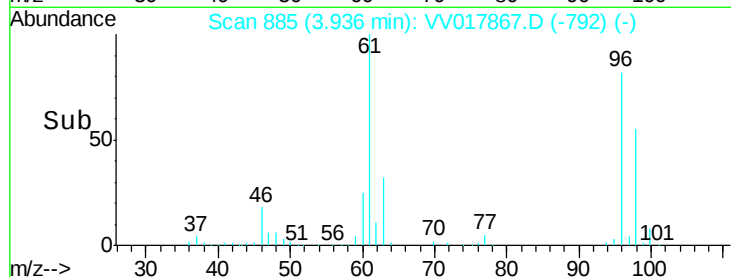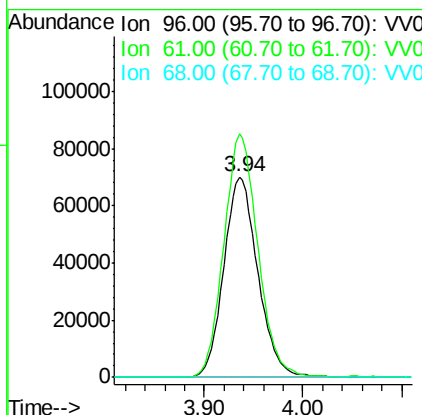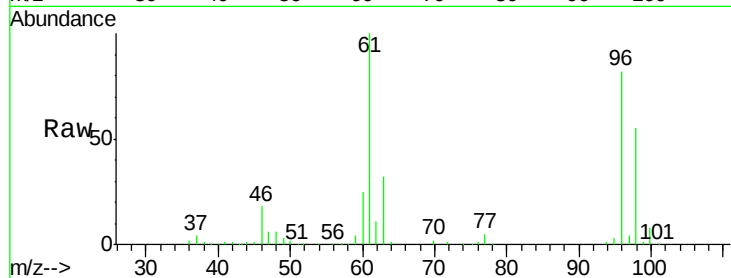

#34
Trichloroethene
Concen: 0.947 ug/L m
RT: 5.94 min Scan# 1508
Delta R.T. 0.00 min
Lab File: VV017867.D
Acq: 08 Aug 2020 20:32

Tgt Ion	Ion	Ratio	Resp	Lower	Upper
95	100		1489		
97	63.1	44.7	83.1		
132	105.4	73.6	136.8		
130	88.4	77.6	144.0		

