

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080823\
 Data File : VV031784.D
 Acq On : 08 Aug 2023 09:28
 Operator : SY/MD
 Sample : VV0808WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK351

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV031784.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rVB	94677	103666	11.52%	1.567%
2	1.532	146	153	169	rVB	94047	115111	12.79%	1.740%
3	2.060	308	317	331	rVB	200560	292028	32.45%	4.415%
4	2.452	428	439	450	rVB6	7015	13306	1.48%	0.201%
5	3.822	854	865	900	rBV2	83694	369067	41.01%	5.580%
6	4.256	984	1000	1027	rBV	152576	397803	44.21%	6.015%
7	4.960	1202	1219	1247	rBV2	287544	781145	86.81%	11.811%
8	5.538	1388	1399	1419	rBV	213344	447323	49.71%	6.763%
9	5.834	1480	1491	1511	rVB6	14776	34603	3.85%	0.523%
10	5.995	1526	1541	1566	rBV	209999	443381	49.27%	6.704%
11	6.921	1818	1829	1851	rBV2	72187	143077	15.90%	2.163%
12	7.249	1919	1931	1952	rBV	277180	500314	55.60%	7.565%
13	7.561	2019	2028	2042	rBV2	48115	91696	10.19%	1.386%
14	8.034	2164	2175	2203	rBV	403647	899836	100.00%	13.605%
15	8.789	2399	2410	2429	rBV	358547	606277	67.38%	9.167%
16	10.159	2825	2836	2849	rBV	161200	263153	29.24%	3.979%
17	11.191	3146	3157	3180	rBV	353916	557093	61.91%	8.423%
18	11.567	3262	3274	3294	rBV	328359	540660	60.08%	8.175%
19	13.451	3851	3860	3869	rBV2	8638	14383	1.60%	0.217%




Sum of corrected areas: 6613922

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080823\
Data File : VV031784.D
Acq On : 08 Aug 2023 09:28
Operator : SY/MD
Sample : VV0808WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK351

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

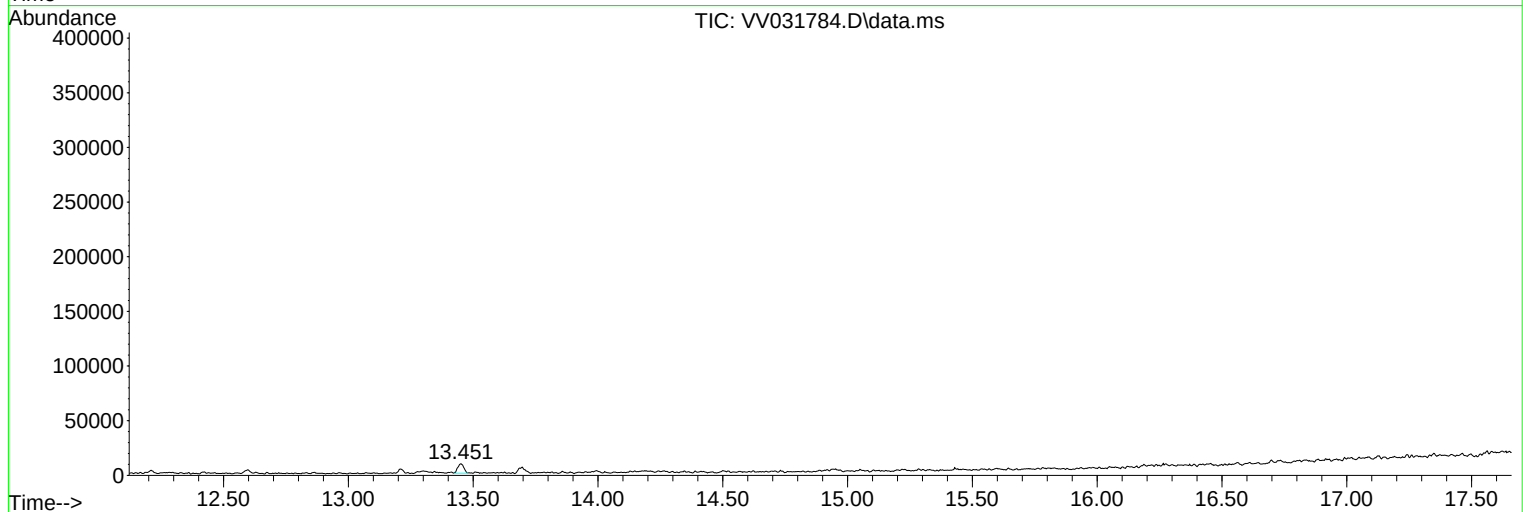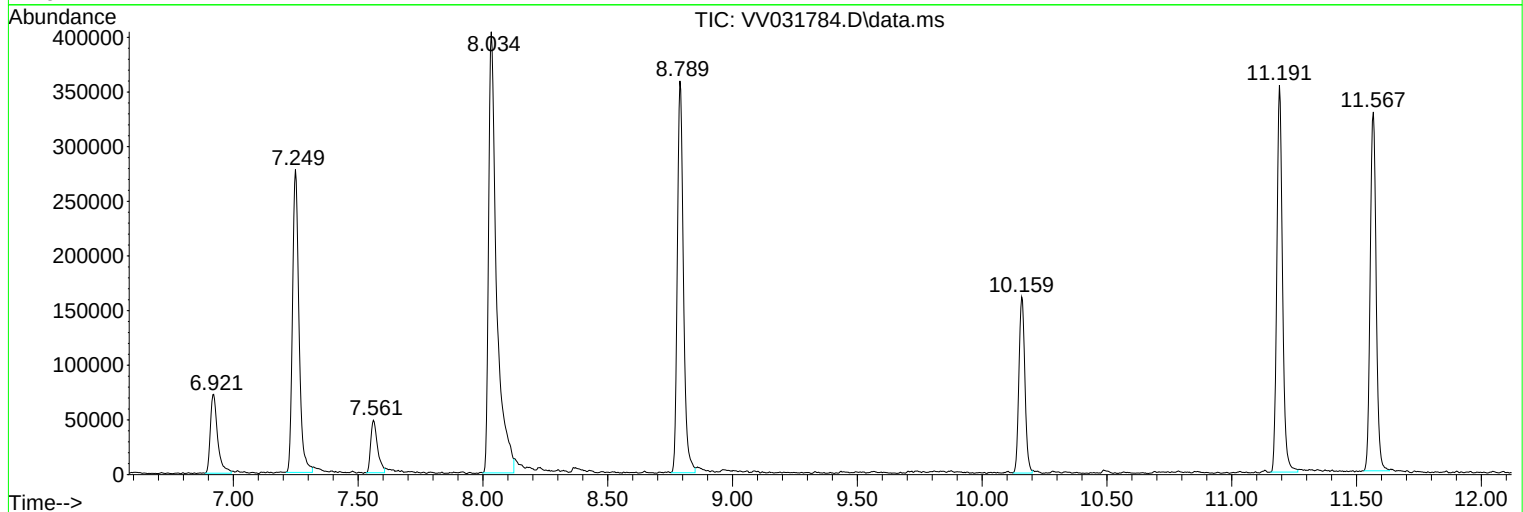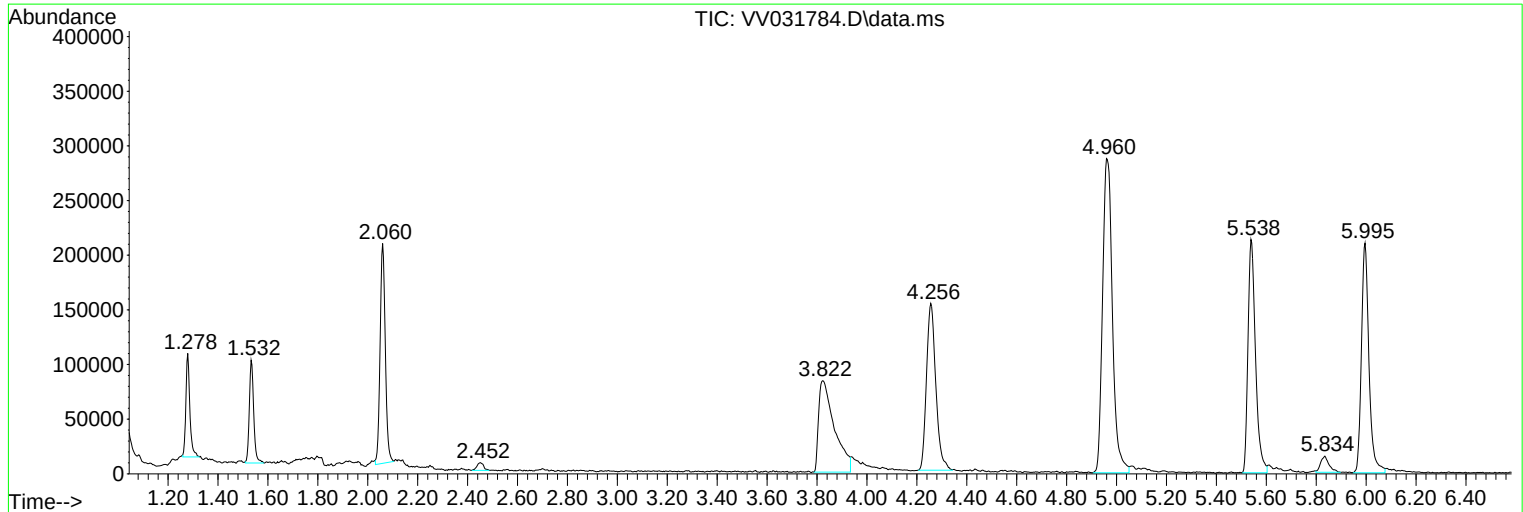

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080823\
Data File : VV031784.D
Acq On : 08 Aug 2023 09:28
Operator : SY/MD
Sample : VV0808WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK351

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080823\
Data File : VV031784.D
Acq On : 08 Aug 2023 09:28
Operator : SY/MD
Sample : VV0808WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK351

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc