

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080823\
 Data File : VV031785.D
 Acq On : 08 Aug 2023 10:05
 Operator : SY/MD
 Sample : 03889-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AF3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV031785.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	93	rVB	102409	119062	14.31%	1.927%
2	1.532	145	153	164	rBV	94290	111362	13.38%	1.803%
3	2.059	307	317	334	rBV	172831	254390	30.57%	4.118%
4	2.449	426	438	454	rVB3	26137	43844	5.27%	0.710%
5	3.825	856	866	898	rBV2	64686	300247	36.08%	4.860%
6	4.252	984	999	1024	rBV2	145438	391288	47.02%	6.334%
7	4.960	1204	1219	1242	rBV2	290156	754266	90.65%	12.210%
8	5.538	1388	1399	1423	rBV2	207402	451839	54.30%	7.314%
9	5.828	1477	1489	1504	rBV3	20059	43499	5.23%	0.704%
10	5.992	1527	1540	1558	rBV	186015	400847	48.17%	6.489%
11	6.921	1819	1829	1849	rBV	56498	112683	13.54%	1.824%
12	7.249	1916	1931	1949	rBV	261096	485739	58.38%	7.863%
13	7.561	2017	2028	2043	rBV2	36399	72145	8.67%	1.168%
14	8.037	2164	2176	2211	rBV2	331067	832098	100.00%	13.470%
15	8.789	2399	2410	2430	rBV	356062	606649	72.91%	9.820%
16	10.159	2825	2836	2852	rBV	131837	216663	26.04%	3.507%
17	10.329	2879	2889	2898	rVB10	5579	11307	1.36%	0.183%
18	11.191	3143	3157	3174	rBV	320070	505420	60.74%	8.182%
19	11.567	3261	3274	3290	rBV	284879	464030	55.77%	7.512%




Sum of corrected areas: 6177378

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080823\
Data File : VV031785.D
Acq On : 08 Aug 2023 10:05
Operator : SY/MD
Sample : 03889-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

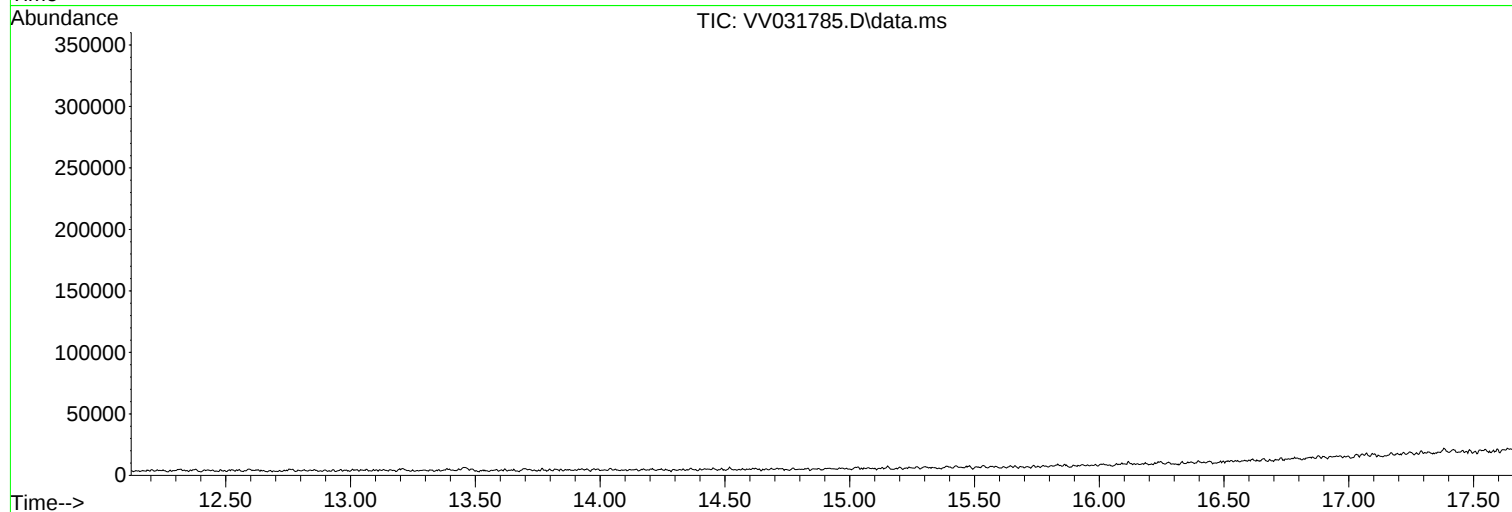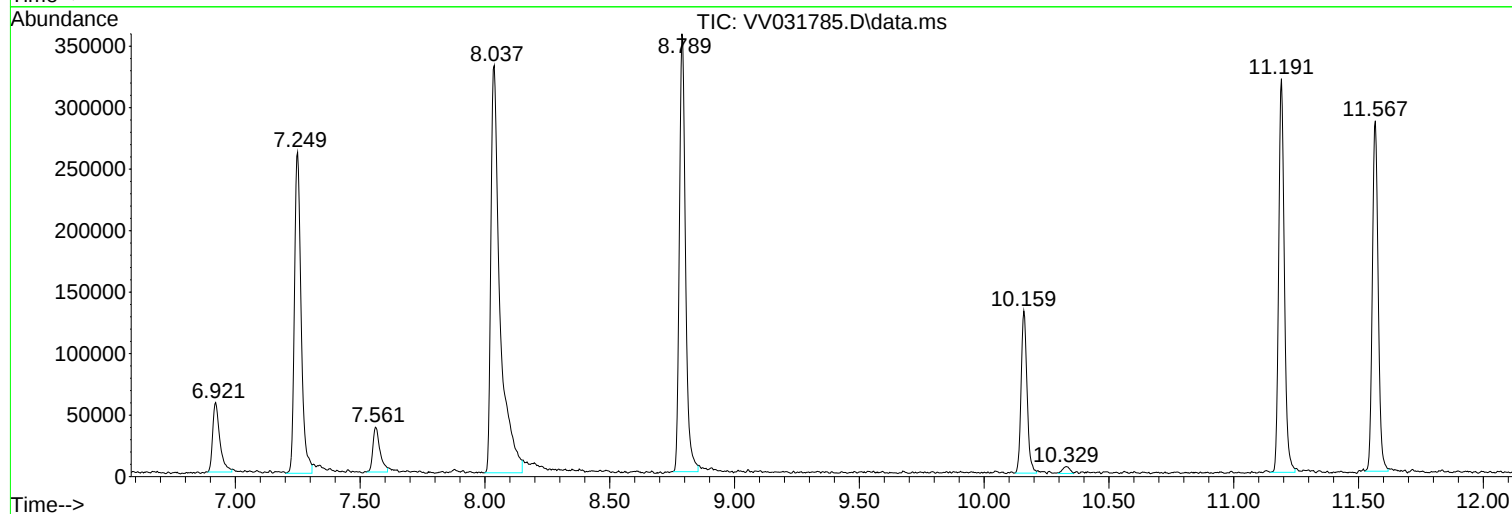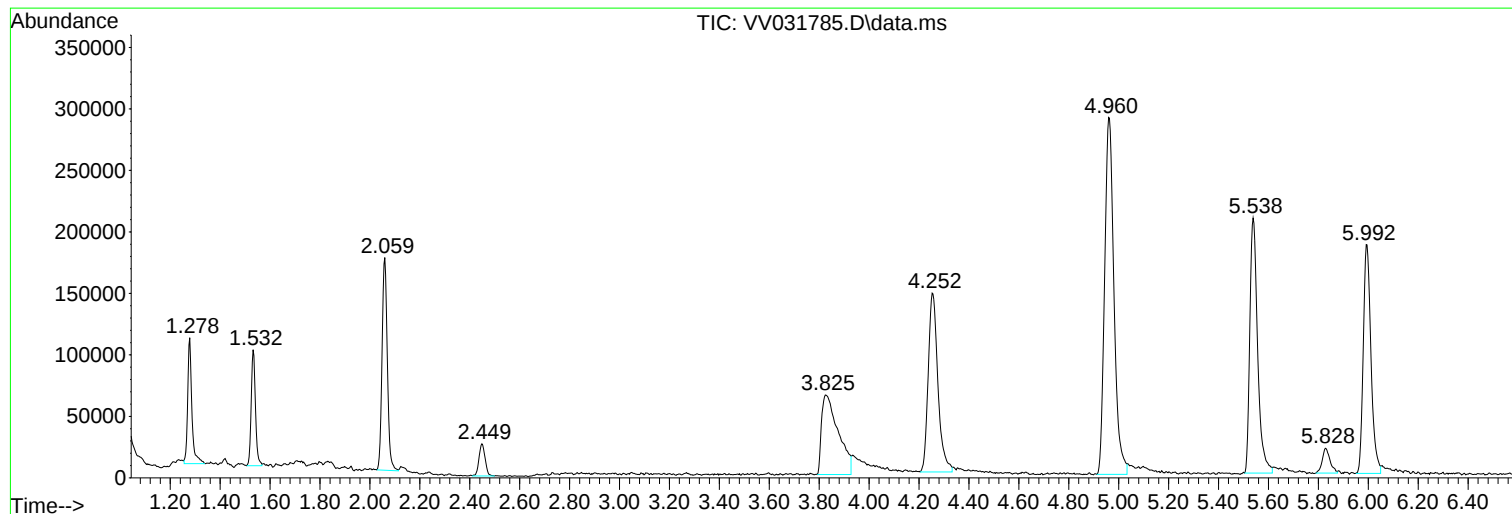

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080823\
Data File : VV031785.D
Acq On : 08 Aug 2023 10:05
Operator : SY/MD
Sample : 03889-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080823\
Data File : VV031785.D
Acq On : 08 Aug 2023 10:05
Operator : SY/MD
Sample : 03889-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc