

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080823\
 Data File : VV031787.D
 Acq On : 08 Aug 2023 15:02
 Operator : SY/MD
 Sample : VIBLK304
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK304

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV031787.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	66	74	90	rVB	86865	96320	10.27%	1.508%
2	1.532	145	153	164	rBV	85487	100736	10.74%	1.577%
3	2.060	305	317	330	rBV	166549	247211	26.36%	3.869%
4	2.449	425	438	450	rBV2	35785	62169	6.63%	0.973%
5	3.828	854	867	891	rBV2	72667	302978	32.30%	4.742%
6	4.256	983	1000	1030	rBV	152085	408078	43.51%	6.387%
7	4.963	1204	1220	1247	rBV3	288766	752466	80.22%	11.778%
8	5.539	1388	1399	1423	rBV	205819	437958	46.69%	6.855%
9	5.834	1480	1491	1502	rBV7	13894	31231	3.33%	0.489%
10	5.995	1527	1541	1562	rBV	196370	425051	45.32%	6.653%
11	6.918	1819	1828	1848	rBV2	63549	128785	13.73%	2.016%
12	7.249	1918	1931	1957	rBV	252926	476473	50.80%	7.458%
13	7.561	2019	2028	2045	rBV2	40411	80012	8.53%	1.252%
14	8.034	2165	2175	2220	rBV	382524	937969	100.00%	14.681%
15	8.789	2399	2410	2433	rBV	358726	616069	65.68%	9.643%
16	10.159	2822	2836	2852	rBV2	161037	262672	28.00%	4.111%
17	11.191	3146	3157	3178	rBV	322301	511098	54.49%	8.000%
18	11.567	3262	3274	3295	rBV2	302828	493930	52.66%	7.731%
19	16.429	4779	4786	4798	rVB7	10139	17698	1.89%	0.277%




Sum of corrected areas: 6388904

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080823\
Data File : VV031787.D
Acq On : 08 Aug 2023 15:02
Operator : SY/MD
Sample : VIBLK304
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK304

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

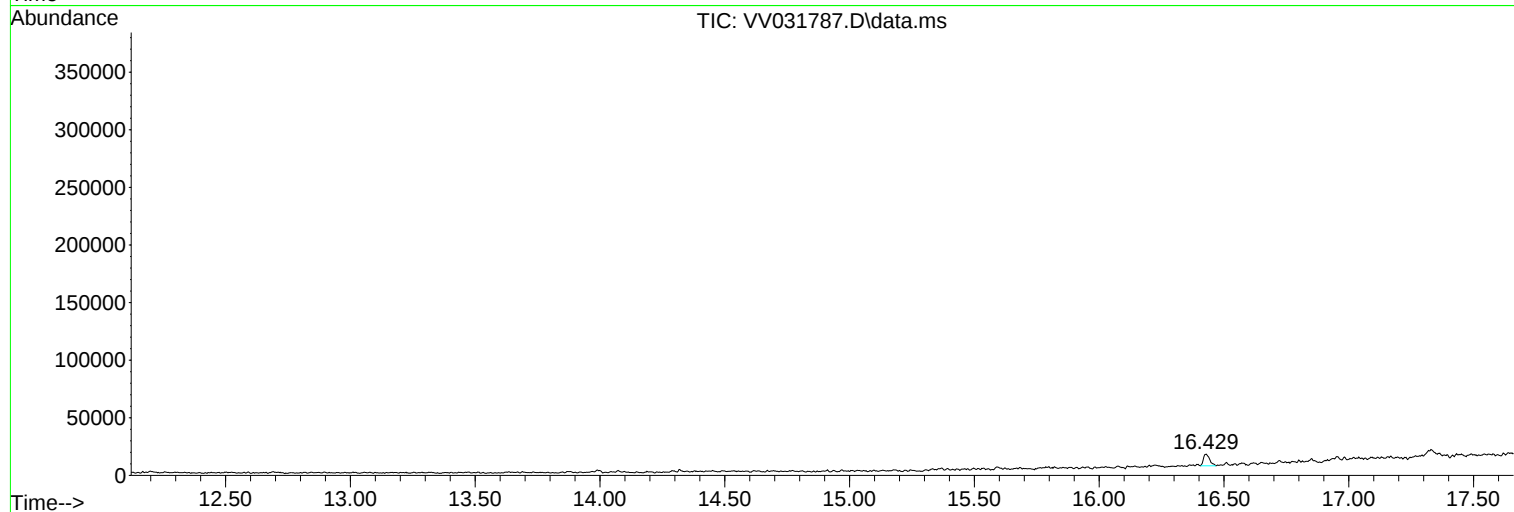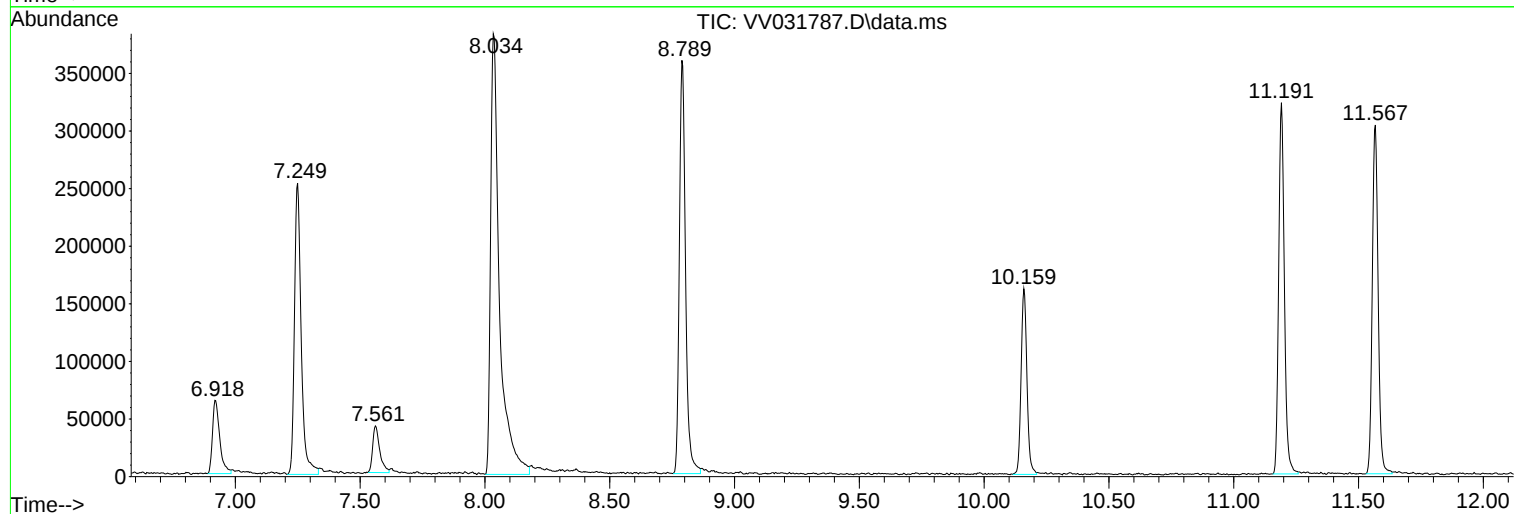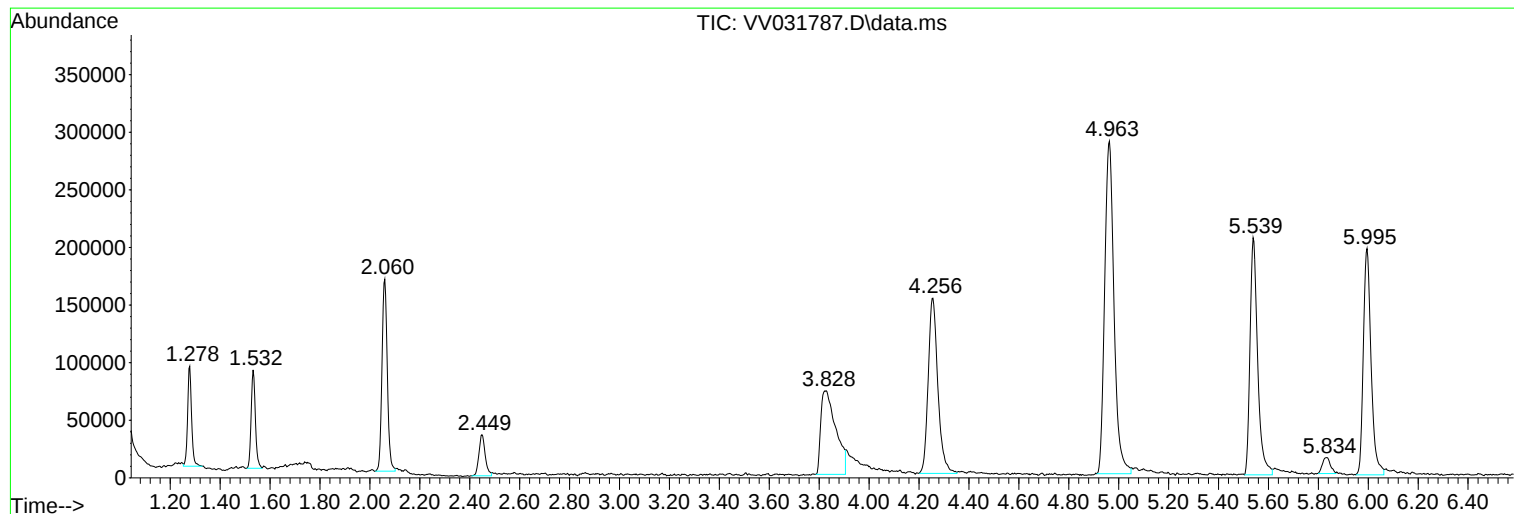

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080823\
Data File : VV031787.D
Acq On : 08 Aug 2023 15:02
Operator : SY/MD
Sample : VIBLK304
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK304

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080823\
Data File : VV031787.D
Acq On : 08 Aug 2023 15:02
Operator : SY/MD
Sample : VIBLK304
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK304

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------