


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080823\
Data File : VV031782.D
Acq On : 08 Aug 2023 08:27
Operator : SY/MD
Sample : BFB284
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB284

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071323WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Jul 18 06:24:32 2023

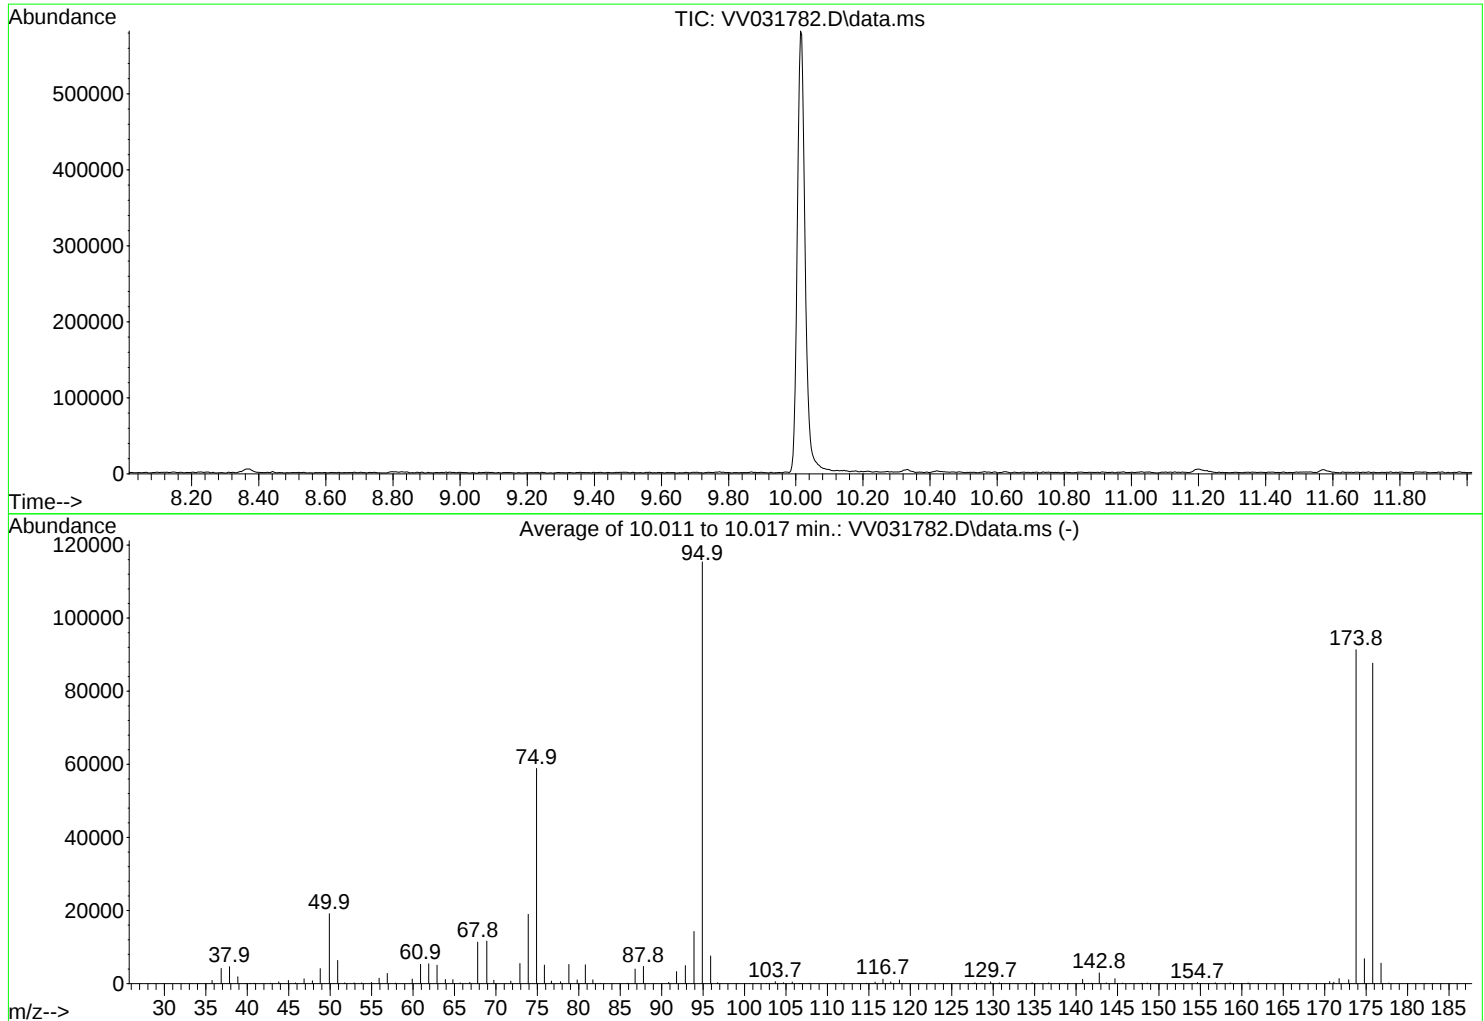

AutoFind: Scans 2790, 2791, 2792; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	19149	PASS
75	95	30	80	51.0	58875	PASS
95	95	100	100	100.0	115392	PASS
96	95	5	9	6.6	7567	PASS
173	174	0.00	2	1.2	1062	PASS
174	95	50	120	79.2	91357	PASS
175	174	5	9	7.5	6836	PASS
176	174	95	105	96.0	87669	PASS
177	176	5	10	6.4	5586	PASS

m/z	Abundance
36.70	118.0
38.30	129.0
39.80	483.0
42.00	182.0
43.80	875.0
51.70	110.0
52.50	101.0
76.70	114.0
134.30	109.0
281.10	130.0

Instrument :
MSVOA_V
ClientSampleId :
BFB284

m/z	Abundance
35.80	810.0
36.90	4131.0
37.90	4421.0
38.90	1795.0
39.80	591.0
40.80	188.0
42.80	129.0
43.80	1190.0
45.00	803.0
45.80	247.0
46.80	1124.0
47.90	778.0
48.80	3913.0
49.90	18480.0
50.90	5989.0
51.80	301.0
52.90	219.0
53.80	199.0
55.00	286.0
55.90	1562.0
56.90	2810.0
57.90	188.0
59.90	1142.0
60.90	5198.0
61.90	5069.0
62.90	4723.0
63.90	1173.0
64.80	972.0
65.70	177.0
66.80	378.0
67.80	10937.0
68.90	10633.0
69.80	913.0
71.80	637.0
72.90	5304.0
73.90	17456.0
74.90	56704.0
75.90	4764.0
76.70	687.0
77.70	506.0
78.80	5182.0
79.70	966.0
80.80	4887.0
81.70	1036.0
82.60	182.0
86.80	3744.0
87.80	4704.0
90.80	338.0
91.80	3218.0
92.80	5211.0
93.90	13181.0
94.90	110192.0
95.90	7067.0
96.70	257.0
103.70	608.0
104.70	275.0
105.80	421.0
106.60	133.0
107.70	104.0
111.70	144.0
114.70	141.0
115.70	454.0
116.70	1145.0
117.70	451.0
118.70	843.0
127.60	264.0
128.60	148.0
129.70	565.0
130.70	234.0
134.70	186.0
136.70	245.0
138.60	138.0
139.10	103.0
140.00	149.0
140.80	1203.0
141.50	108.0
141.90	122.0
142.80	2797.0
143.70	199.0
144.70	1249.0
145.60	129.0
147.90	191.0
148.60	165.0
149.60	131.0
152.70	114.0
154.60	297.0
156.80	252.0
158.60	210.0
160.80	263.0
170.60	519.0
171.10	342.0
171.70	1332.0

Instrument :
MSVOA_V
ClientSampleId :
BFB284

173.80	84776.0
174.80	6306.0
175.80	80864.0
176.80	5267.0
177.80	137.0

Instrument :
MSVOA_V
ClientSampleId :
BFB284

m/z	Abundance
35.70	869.0
36.90	4451.0
37.80	4879.0
38.90	1954.0
39.80	552.0
40.80	169.0
41.90	111.0
42.80	113.0
43.80	1377.0
44.90	911.0
45.80	236.0
46.80	1380.0
47.90	858.0
48.80	4240.0
49.90	19800.0
50.90	6437.0
51.80	308.0
52.90	219.0
53.80	249.0
55.00	359.0
55.90	1488.0
56.90	2874.0
57.90	189.0
59.90	1328.0
60.90	5437.0
61.90	5637.0
62.90	5114.0
63.90	1212.0
64.80	1113.0
65.70	236.0
66.90	367.0
67.80	11690.0
68.90	12053.0
69.70	931.0
71.80	717.0
72.90	5718.0
73.90	19560.0
74.90	60976.0
75.90	5115.0
76.80	801.0
77.80	558.0
78.80	5336.0
79.80	991.0
80.80	5290.0
81.70	1144.0
82.60	123.0
85.90	198.0
86.80	4163.0
87.80	4911.0
90.90	353.0
91.80	3340.0
92.80	5010.0
93.90	14886.0
94.90	119136.0
95.90	7897.0
96.80	284.0
99.20	101.0
102.60	121.0
103.70	634.0
104.70	262.0
105.80	527.0
106.80	113.0
107.80	122.0
111.70	131.0
114.70	126.0
115.80	430.0
116.70	1260.0
117.70	482.0
118.70	1067.0
127.80	296.0
128.70	194.0
129.70	522.0
130.70	198.0
134.70	273.0
136.70	219.0
138.70	101.0
140.80	1186.0
141.90	112.0
142.80	3137.0
143.60	215.0
144.70	1397.0
145.60	155.0
147.90	178.0
148.60	180.0
149.70	156.0
154.70	323.0
156.80	288.0
158.60	221.0
160.70	236.0
170.60	632.0
171.10	418.0
171.80	1463.0

Instrument :
MSVOA_V
ClientSampleId :
BFB284

172.90	1529.0
173.80	94704.0
174.80	6961.0
175.80	90496.0
176.80	5776.0
177.70	167.0

Instrument :
MSVOA_V
ClientSampleId :
BFB284

m/z	Abundance
35.70	905.0
36.90	4271.0
37.80	4606.0
38.80	1892.0
39.70	481.0
40.40	247.0
41.90	133.0
42.80	107.0
43.80	1549.0
44.90	981.0
45.80	230.0
46.90	1457.0
47.80	786.0
48.80	4196.0
49.90	19168.0
50.90	6653.0
51.80	366.0
52.90	243.0
53.80	261.0
55.00	376.0
55.90	1415.0
56.90	2720.0
57.90	209.0
59.90	1285.0
60.90	5247.0
61.90	5595.0
62.90	5220.0
63.90	1075.0
64.80	1150.0
65.70	213.0
66.80	351.0
67.80	11376.0
68.90	12225.0
69.80	952.0
71.80	787.0
72.90	5544.0
73.90	19840.0
74.90	58944.0
75.80	5358.0
76.80	987.0
77.90	503.0
78.80	5234.0
79.90	1056.0
80.80	5338.0
81.70	985.0
85.80	217.0
86.80	4068.0
87.80	4543.0
90.90	382.0
91.80	3326.0
92.90	4615.0
93.90	14729.0
94.90	116848.0
95.90	7738.0
96.80	255.0
102.70	141.0
103.70	532.0
104.70	229.0
105.70	570.0
106.80	139.0
107.90	199.0
110.80	121.0
111.70	123.0
114.70	136.0
115.80	459.0
116.70	1261.0
117.60	483.0
118.70	1117.0
122.30	105.0
123.50	102.0
127.80	328.0
128.70	175.0
129.70	432.0
130.80	178.0
134.70	278.0
136.70	193.0
140.80	1198.0
141.80	127.0
142.80	2925.0
143.70	252.0
144.70	1447.0
145.70	196.0
146.50	119.0
147.60	176.0
148.60	160.0
149.70	155.0
154.70	299.0
156.80	248.0
158.60	218.0
160.70	209.0
170.60	629.0
171.10	460.0

Instrument :
MSVOA_V
ClientSampleId :
BFB284

171.80	1461.0
172.90	1656.0
173.80	94592.0
174.80	7241.0
175.80	91648.0
176.80	5716.0
177.70	209.0

Instrument :
MSVOA_V
ClientSampleId :
BFB284