


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV080825\
Data File : VV038925.D
Acq On : 08 Aug 2025 08:07
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\82V080825W.M
Title : SW846 8260
Last Update : Mon Aug 11 05:27:06 2025

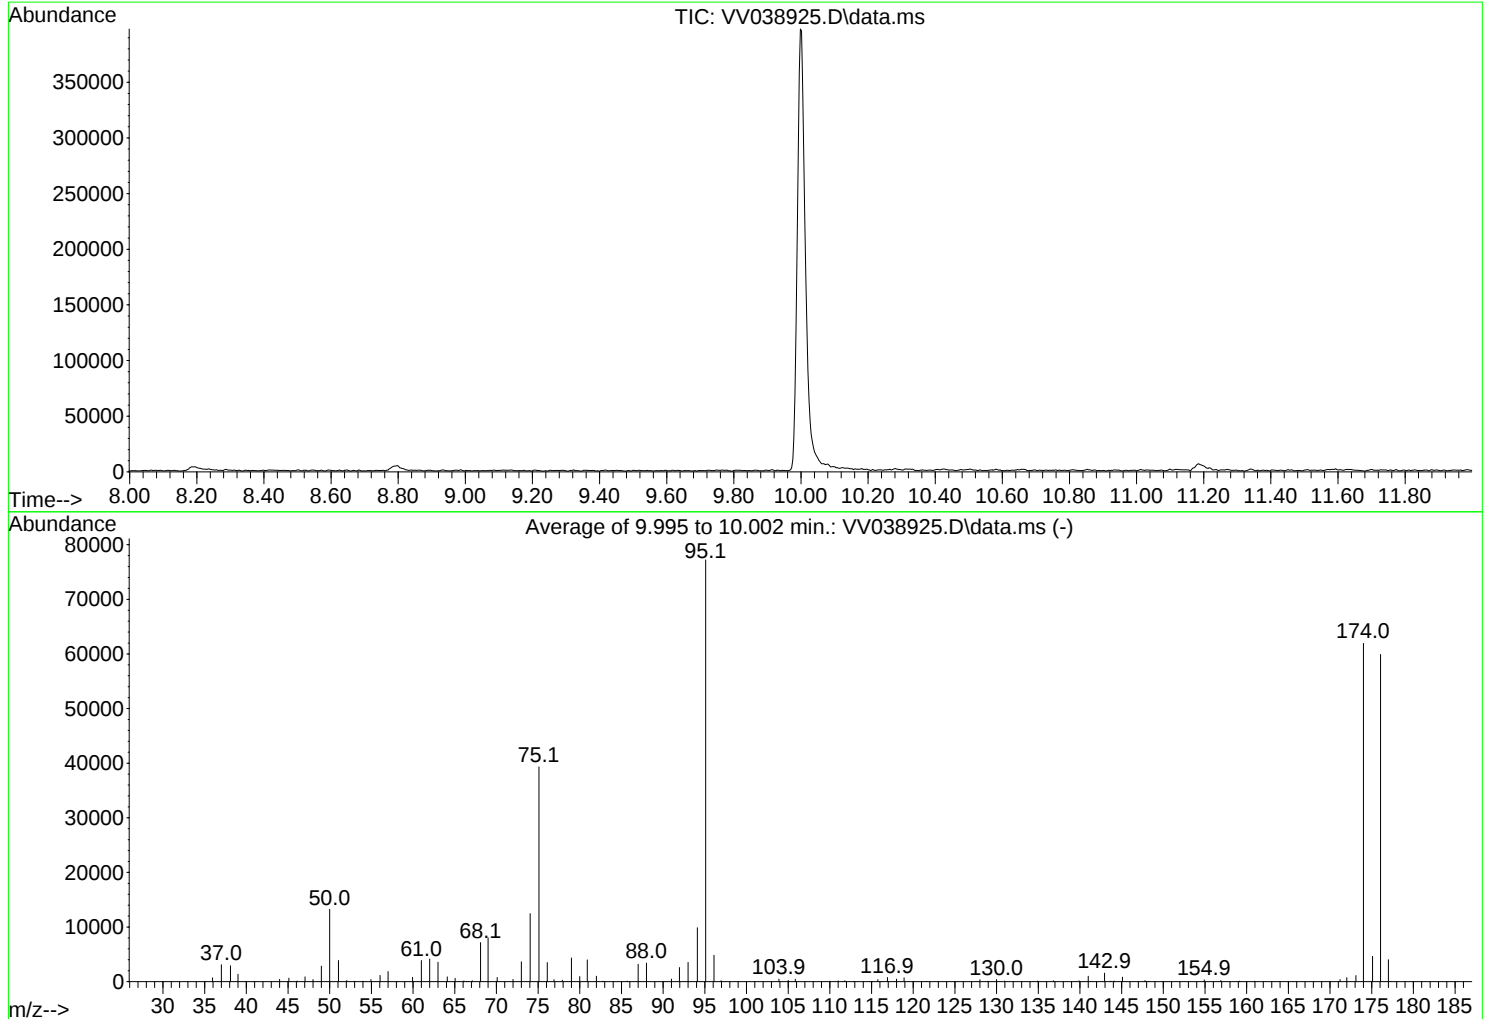

AutoFind: Scans 2785, 2786, 2787; Background Corrected with Scan 2774

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	13235	PASS
75	95	30	60	50.9	39304	PASS
95	95	100	100	100.0	77229	PASS
96	95	5	9	6.2	4822	PASS
173	174	0.00	2	1.8	1124	PASS
174	95	50	100	80.2	61947	PASS
175	174	5	9	7.5	4645	PASS
176	174	95	101	96.7	59912	PASS
177	176	5	9	6.7	4023	PASS