

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV080918\
 Data File : VV006961.D
 Acq On : 09 Aug 2018 20:00
 Operator : SY/MD
 Sample : J4357-02RE
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ESWS1RE

Quant Time: Aug 10 03:03:42 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080918WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Aug 10 02:34:57 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	240969	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	231686	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	91031	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	75672	4.86	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	97.20%
7) Chloroethane-d5	1.58	69	65890	4.99	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	99.80%
11) 1,1-Dichloroethene-d2	2.13	63	99783	3.42	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	68.40%
20) 2-Butanone-d5	3.97	46	232546	51.99	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	103.98%
24) Chloroform-d	4.41	84	152645	4.84	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.80%
26) 1,2-Dichloroethane-d4	5.09	65	82207	5.16	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.20%
32) Benzene-d6	5.11	84	288295	4.84	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.80%
36) 1,2-Dichloropropane-d6	6.12	67	101704	5.00	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.00%
41) Toluene-d8	7.37	98	214898	4.24	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.80%
43) trans-1,3-Dichloropropene-	7.67	79	30296	4.28	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.60%
46) 2-Hexanone-d5	8.15	63	118258	40.85	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	81.70%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	75305	4.75	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.00%
64) 1,2-Dichlorobenzene-d4	11.68	152	77503	4.89	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.80%

Target Compounds


					Ovalue
13) Acetone	2.21	43	15694	6.81 ug/L	94
22) cis-1,2-Dichloroethene	3.97	96	18448	0.88 ug/L	92
27) 1,2-Dichloroethane	5.19	62	11651	0.51 ug/L	100
34) Trichloroethene	5.96	95	4461	0.23 ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV080918\
Data File : VV006961.D
Acq On : 09 Aug 2018 20:00
Operator : SY/MD
Sample : J4357-02RE
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ESWS1RE

Quant Time: Aug 10 03:03:42 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080918WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Aug 10 02:34:57 2018
Response via : Initial Calibration

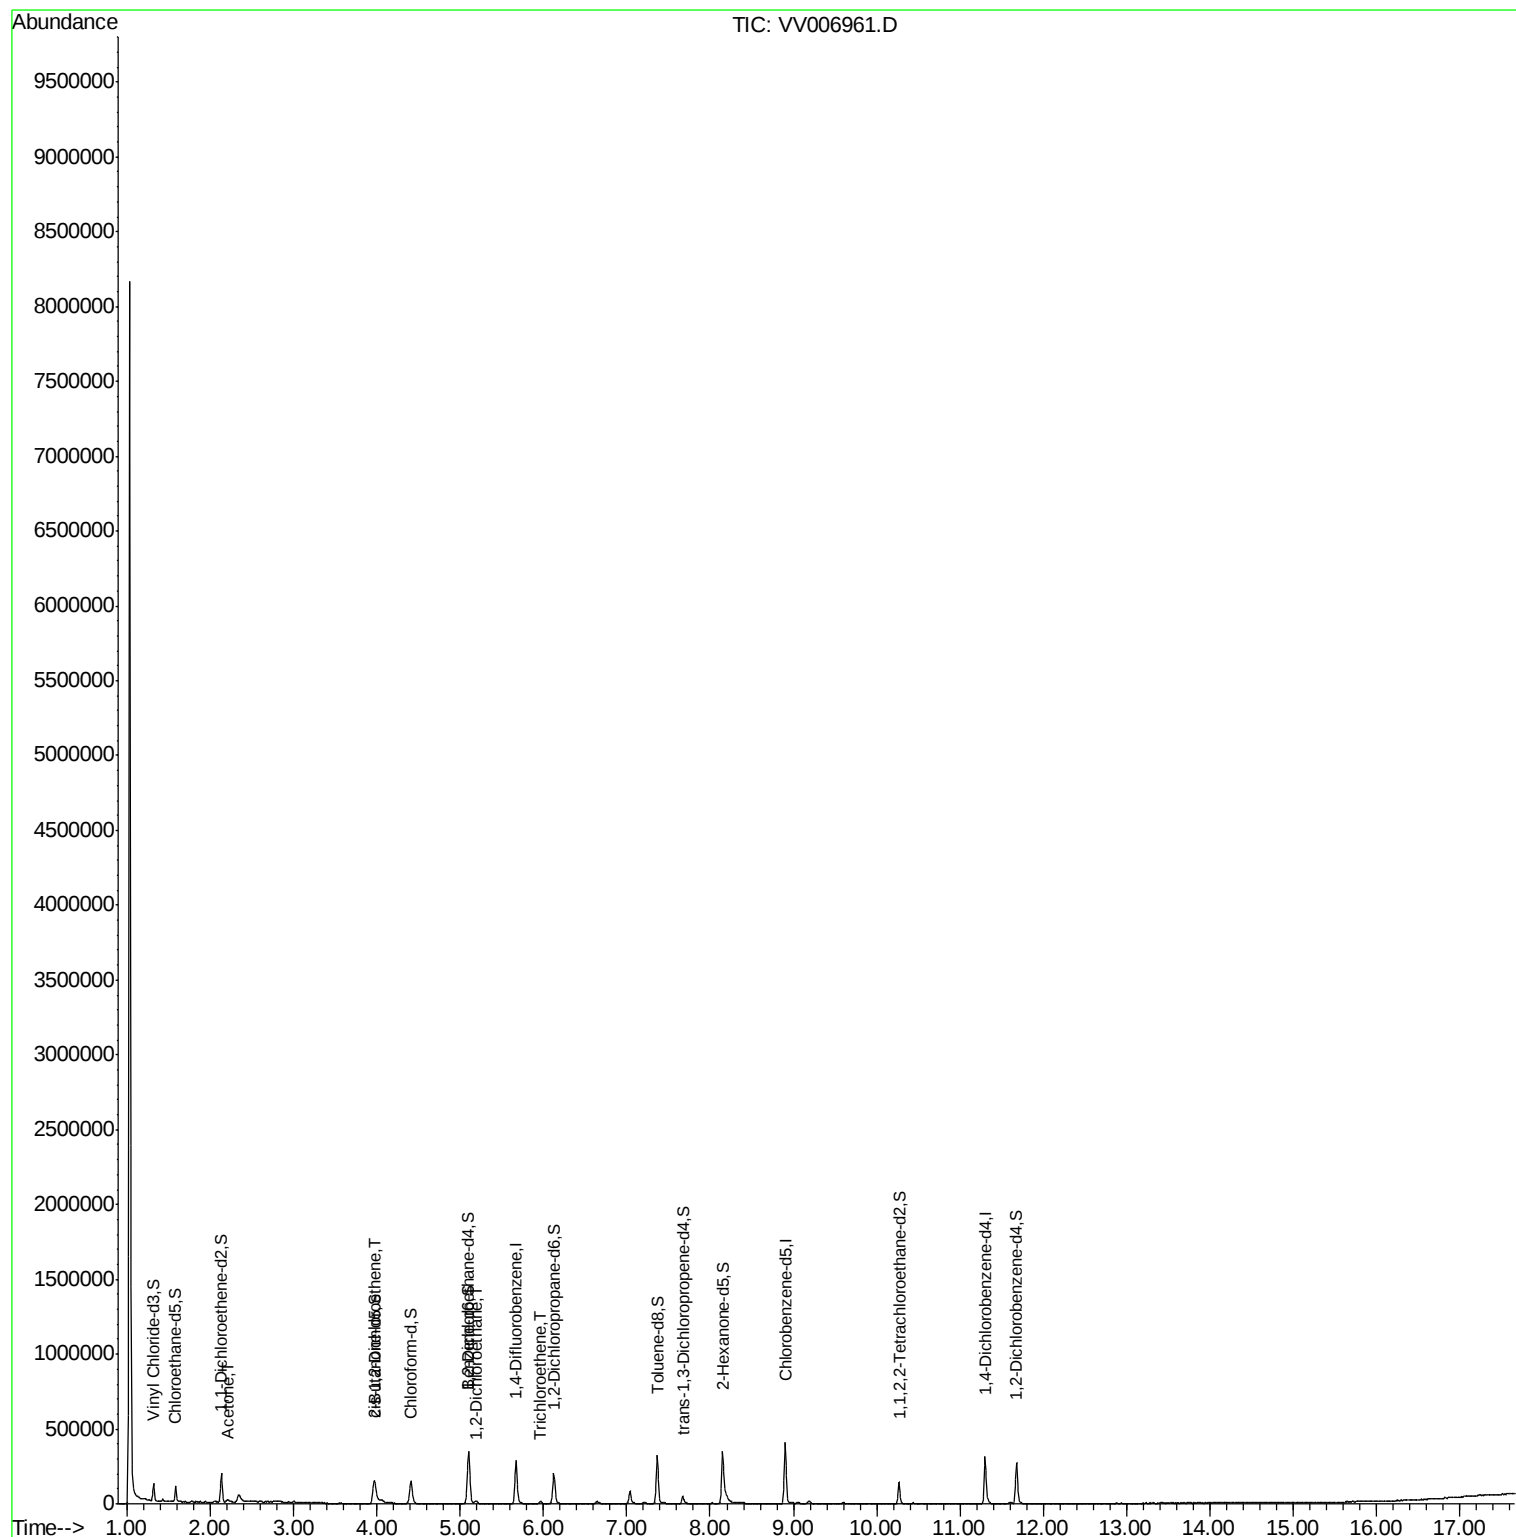

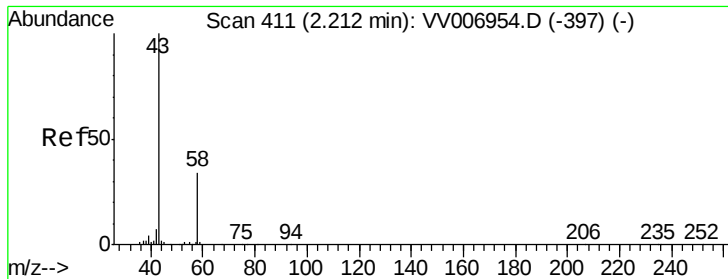

#13

Acetone

Concen: 6.81 ug/L

RT: 2.21 min Scan# 409

Delta R.T. -0.01 min

Lab File: VV006961.D

Acq: 09 Aug 2018 20:00

Instrument :

MSVOA_V

ClientSampleId :


ESWS1RE

Tot Ion: 43 Resp: 15694

Ion Ratio Lower Upper




43 100

58 39.4 0.0 71.4

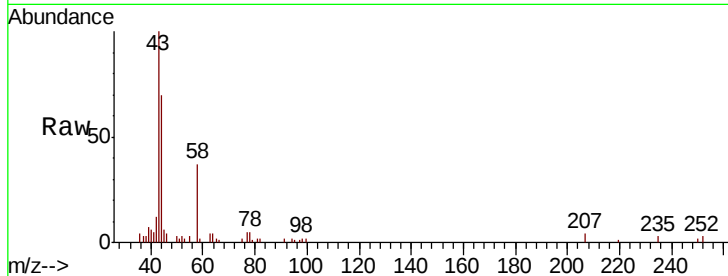

Abundance Ion 43.05 (42.75 to 43.75): VV006954.D (-397) (-)

Ion 58.05 (57.75 to 58.75): VV006954.D (-397) (-)

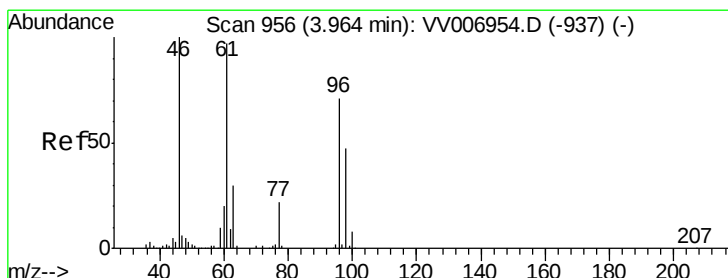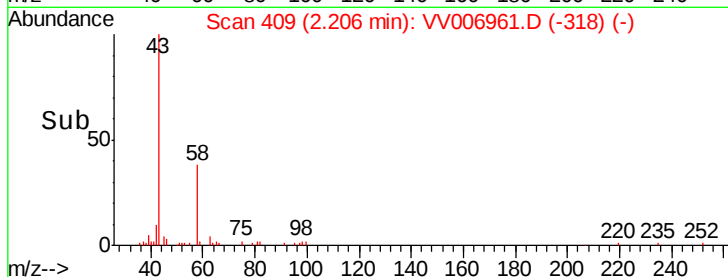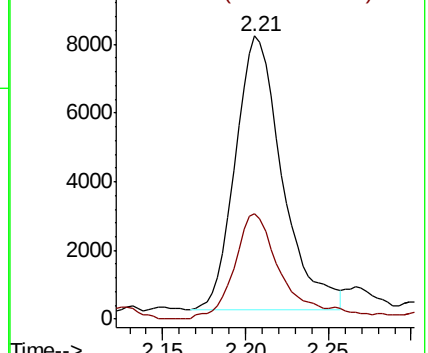

#22

cis-1,2-Dichloroethene

Concen: 0.88 ug/L

RT: 3.97 min Scan# 958

Delta R.T. 0.01 min

Lab File: VV006961.D

Acq: 09 Aug 2018 20:00


Tgt Ion: 96 Resp: 18448

Ion Ratio Lower Upper

96 100

61 139.2 91.1 169.1



68 0.0 0.0 0.0

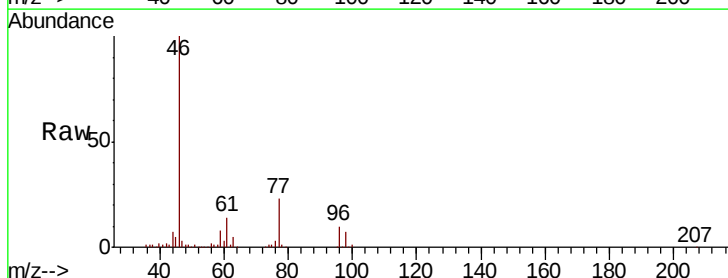


Abundance Ion 96.00 (95.70 to 96.70): VV006954.D (-937) (-)

Ion 61.05 (60.75 to 61.75): VV006954.D (-937) (-)

Ion 68.15 (67.85 to 68.85): VV006954.D (-937) (-)

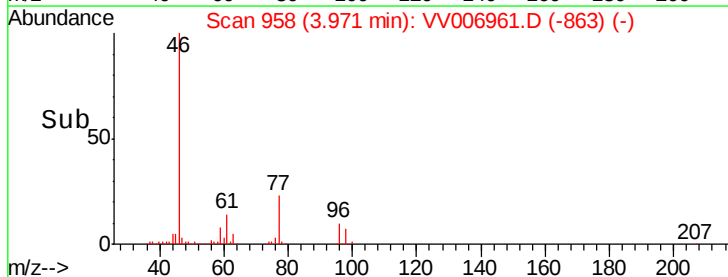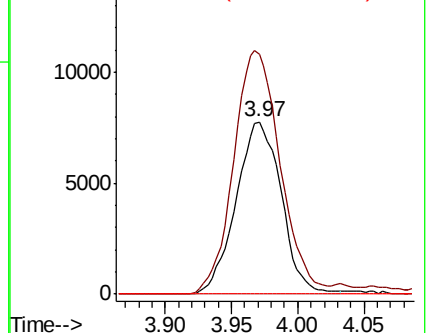

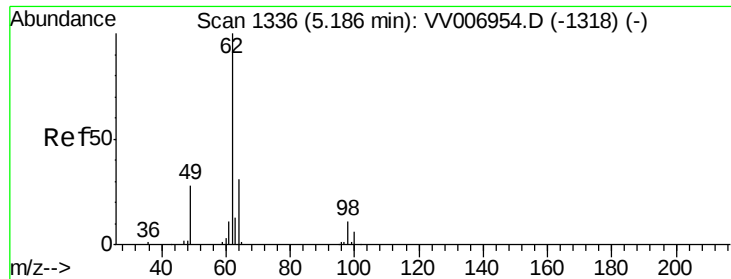

#27

1,2-Dichloroethane

Concen: 0.51 ug/L

RT: 5.19 min Scan# 1337

Delta R.T. 0.00 min

Lab File: VV006961.D

Acq: 09 Aug 2018 20:00

Instrument :

MSVOA_V

ClientSampleId :


ESWS1RE

Tot Ion: 62 Resp: 11651

Ion Ratio Lower Upper




62 100

98 9.3 7.6 11.4

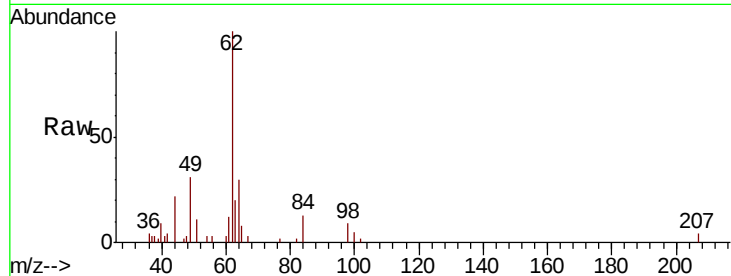

Abundance Ion 62.00 (61.70 to 62.70): VV006961.D (-1243) (-)

Ion 98.05 (97.75 to 98.75): VV006961.D (-1243) (-)

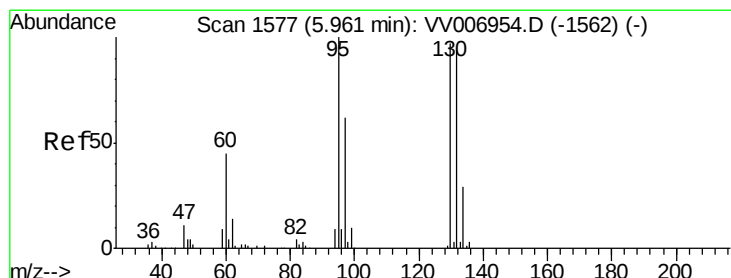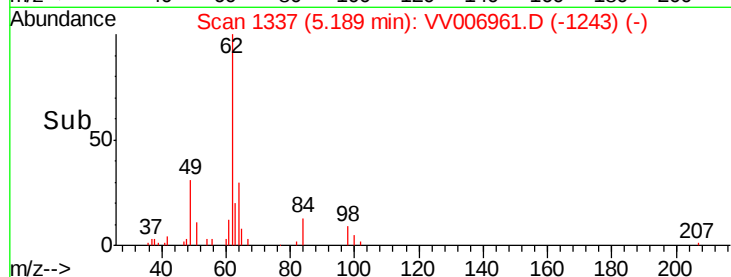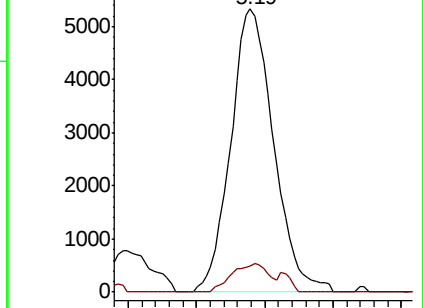

#34

Trichloroethene

Concen: 0.23 ug/L

RT: 5.96 min Scan# 1578

Delta R.T. 0.00 min

Lab File: VV006961.D

Acq: 09 Aug 2018 20:00

Tgt Ion: 95 Resp: 4461


Ion Ratio Lower Upper

95 100

97 58.3 44.8 83.2

132 83.1 65.5 121.6

130 86.8 66.4 123.4

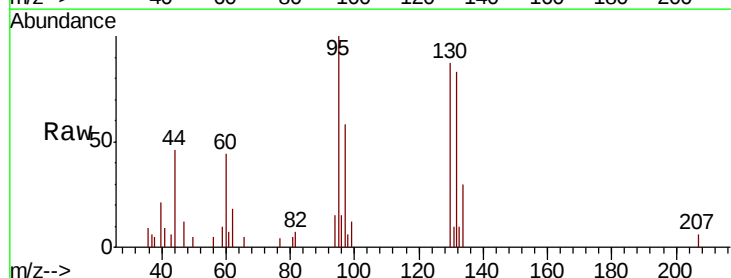

Abundance Ion 95.00 (94.70 to 95.70): VV006961.D (-1484) (-)

Ion 96.95 (96.65 to 97.65): VV006961.D (-1484) (-)

Ion 131.95 (131.65 to 132.65): VV006961.D (-1484) (-)

Ion 129.95 (129.65 to 130.65): VV006961.D (-1484) (-)

