

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV080918\
 Data File : VV006963.D
 Acq On : 09 Aug 2018 21:20
 Operator : SY/MD
 Sample : J4399-01
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BC6R1

Quant Time: Aug 10 09:05:06 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080918WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Aug 10 02:34:57 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	230607	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	218623	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	88215	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	69013	4.64	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	92.80%
7) Chloroethane-d5	1.58	69	64199	5.08	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	101.60%
11) 1,1-Dichloroethene-d2	2.13	63	90426	3.24	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	64.80%
20) 2-Butanone-d5	3.97	46	223252	52.15	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	104.30%
24) Chloroform-d	4.41	84	150221	4.97	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.40%
26) 1,2-Dichloroethane-d4	5.09	65	79461	5.21	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.20%
32) Benzene-d6	5.10	84	285935	5.09	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.80%
36) 1,2-Dichloropropane-d6	6.12	67	99983	5.21	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	104.20%
41) Toluene-d8	7.37	98	208524	4.36	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.20%
43) trans-1,3-Dichloropropene-	7.67	79	30539	4.57	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.40%
46) 2-Hexanone-d5	8.15	63	114764	42.01	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	84.02%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	72730	4.86	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.20%
64) 1,2-Dichlorobenzene-d4	11.68	152	78552	5.12	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.40%


Target Compounds					Ovalue
13) Acetone	2.21	43	59238	26.87 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV080918\
Data File : VV006963.D
Acq On : 09 Aug 2018 21:20
Operator : SY/MD
Sample : J4399-01
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BC6R1

Quant Time: Aug 10 09:05:06 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080918WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Aug 10 02:34:57 2018
Response via : Initial Calibration

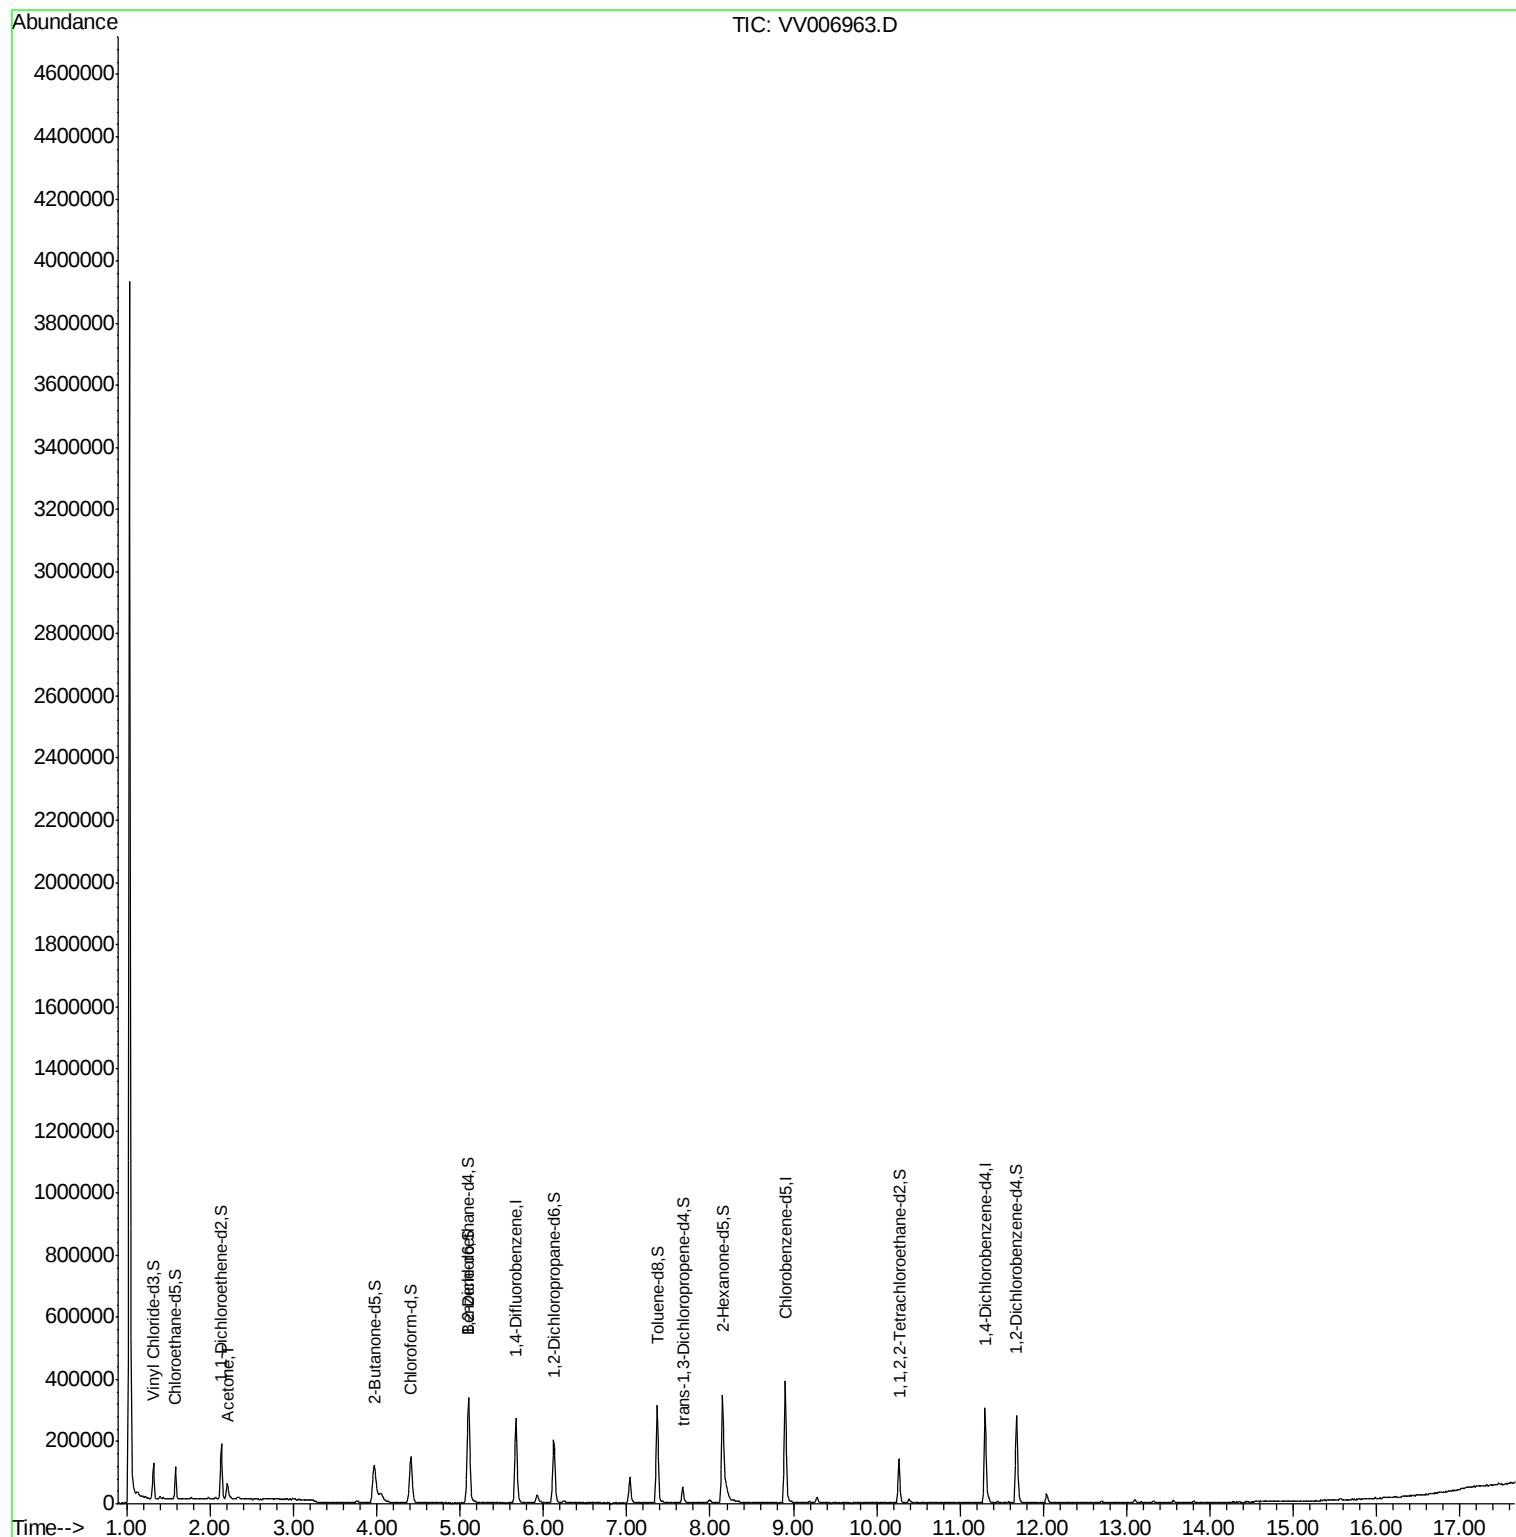

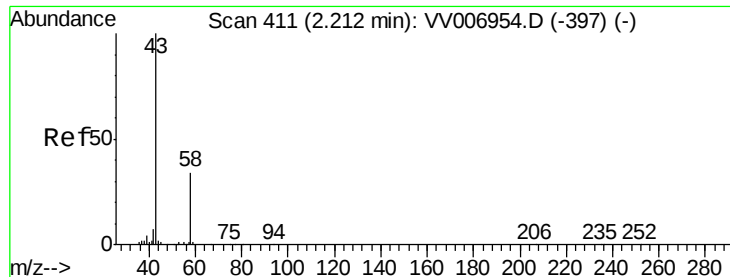

#13

Acetone

Concen: 26.87 ug/L

RT: 2.21 min Scan# 409

Delta R.T. -0.01 min

Lab File: VV006963.D

Acq: 09 Aug 2018 21:20

Instrument :
MSVOA_V
ClientSampleId :
BC6R1

Tot Ion: 43 Resp: 59238

Ion Ratio Lower Upper

43 100

58 33.2 0.0 71.4

