

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV080918\
 Data File : VV006965.D
 Acq On : 09 Aug 2018 22:14
 Operator : SY/MD
 Sample : J4399-03
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BC6R3

Quant Time: Aug 10 03:59:28 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080918WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Aug 10 02:34:57 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	233506	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	222361	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	89729	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	71779	4.76	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	95.20%
7) Chloroethane-d5	1.58	69	65154	5.10	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	102.00%
11) 1,1-Dichloroethene-d2	2.13	63	99970	3.53	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.60%
20) 2-Butanone-d5	3.97	46	226170	52.18	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	104.36%
24) Chloroform-d	4.41	84	154959	5.07	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.40%
26) 1,2-Dichloroethane-d4	5.09	65	81565	5.28	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.60%
32) Benzene-d6	5.10	84	293192	5.13	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.60%
36) 1,2-Dichloropropane-d6	6.12	67	103052	5.28	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	105.60%
41) Toluene-d8	7.37	98	217226	4.47	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.40%
43) trans-1,3-Dichloropropene-	7.67	79	30479	4.49	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.80%
46) 2-Hexanone-d5	8.15	63	120773	43.47	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	86.94%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	74137	4.87	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.40%
64) 1,2-Dichlorobenzene-d4	11.68	152	78929	5.06	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.20%


Target Compounds					Ovalue
13) Acetone	2.21	43	9541	4.27 ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV080918\
Data File : VV006965.D
Acq On : 09 Aug 2018 22:14
Operator : SY/MD
Sample : J4399-03
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BC6R3

Quant Time: Aug 10 03:59:28 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080918WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Aug 10 02:34:57 2018
Response via : Initial Calibration

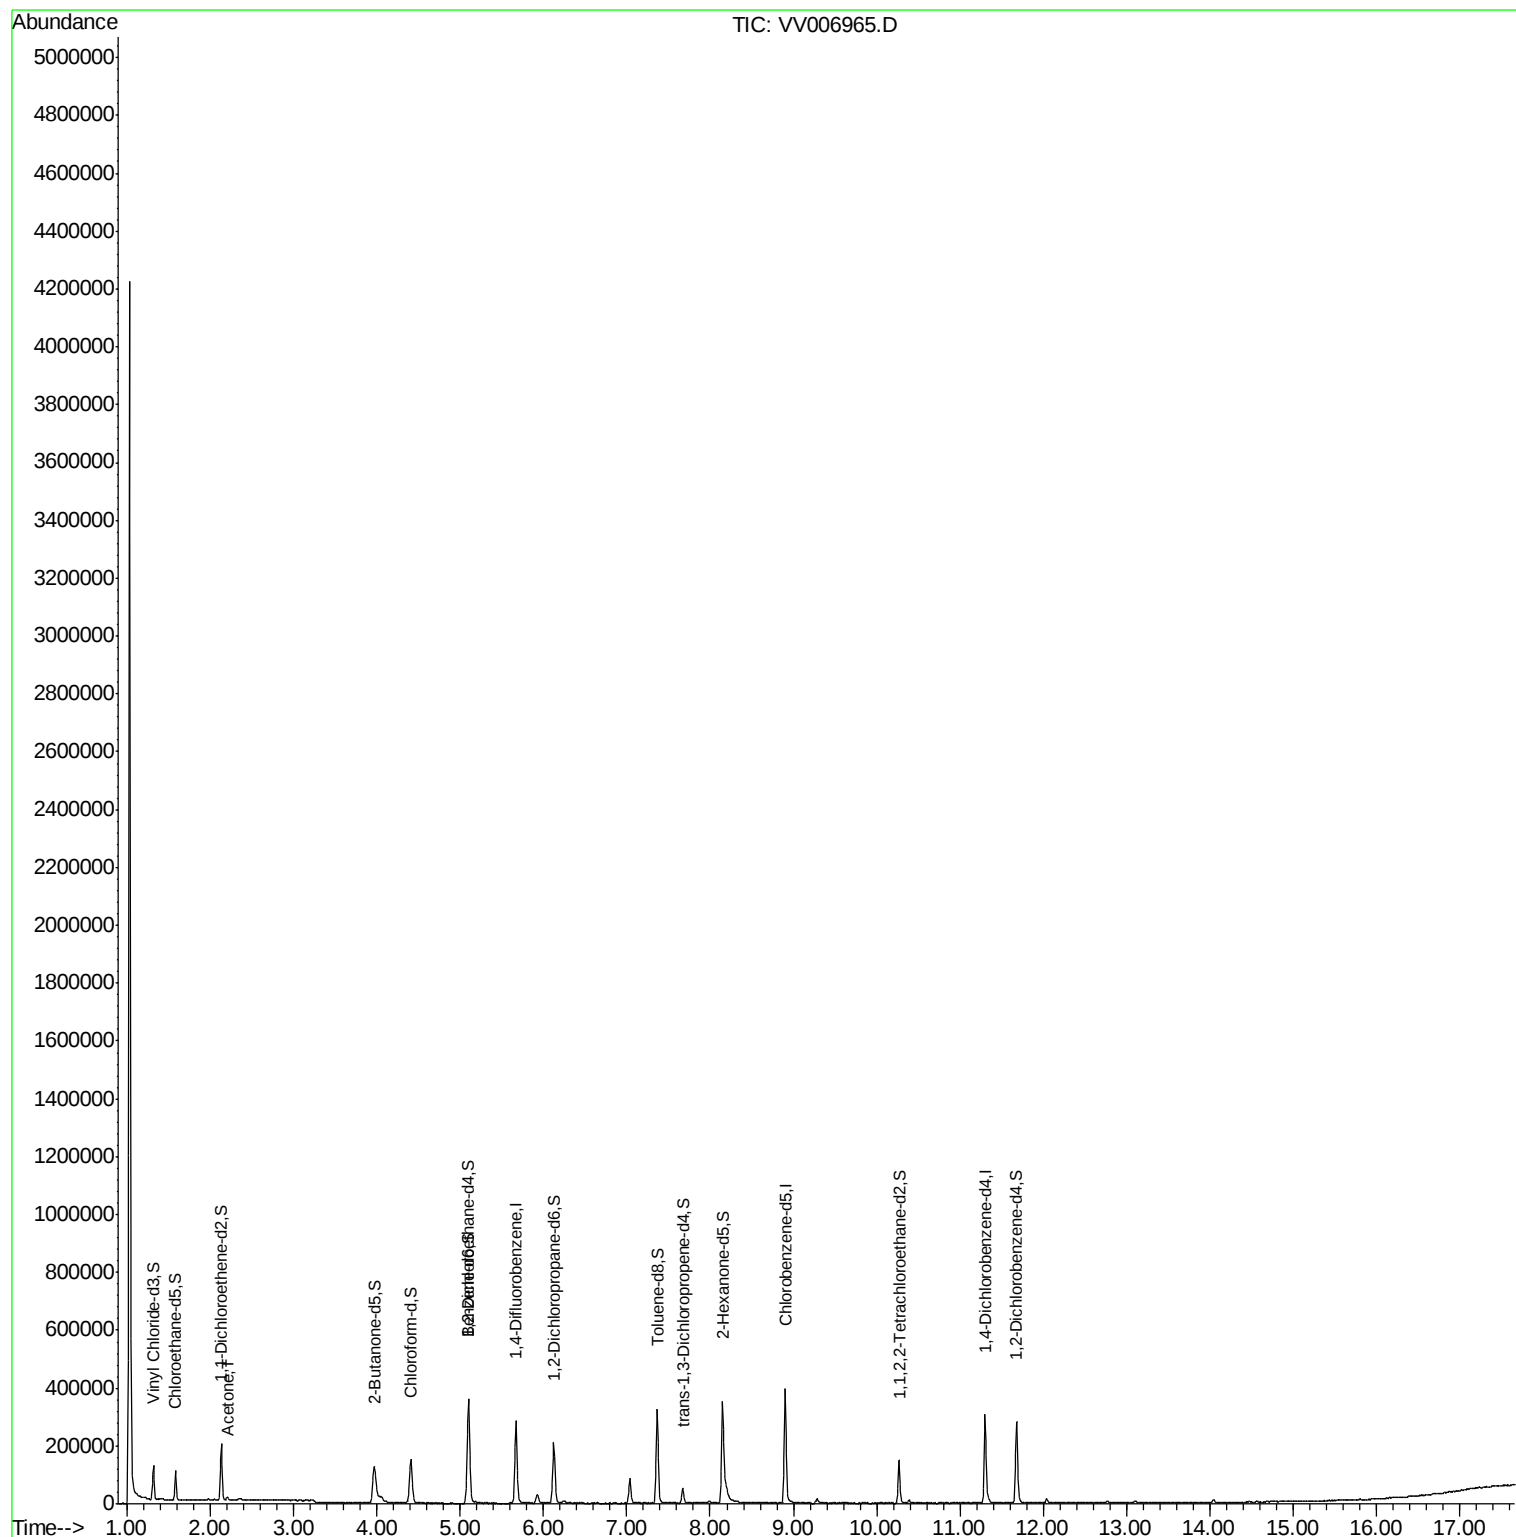

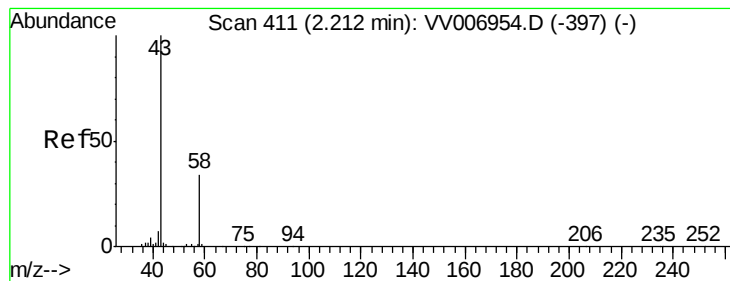

#13

Acetone

Concen: 4.27 ug/L

RT: 2.21 min Scan# 409

Delta R.T. -0.01 min

Lab File: VV006965.D

Acq: 09 Aug 2018 22:14

Instrument :
MSVOA_V
ClientSampleId :
BC6R3

Tot Ion: 43 Resp: 9541

Ion Ratio Lower Upper

43 100

58 42.6 0.0 71.4

