

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV080918\
 Data File : VV006966.D
 Acq On : 09 Aug 2018 22:41
 Operator : SY/MD
 Sample : J4399-04
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BC6R4

Quant Time: Aug 10 04:00:49 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080918WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Aug 10 02:34:57 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	222499	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	213356	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	85055	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	70599	4.92	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	98.40%
7) Chloroethane-d5	1.58	69	64920	5.33	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	106.60%
11) 1,1-Dichloroethene-d2	2.13	63	95883	3.56	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	71.20%
20) 2-Butanone-d5	3.97	46	224270	54.30	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	108.60%
24) Chloroform-d	4.41	84	151125	5.19	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.80%
26) 1,2-Dichloroethane-d4	5.09	65	80500	5.47	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	109.40%
32) Benzene-d6	5.10	84	287038	5.24	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.80%
36) 1,2-Dichloropropane-d6	6.12	67	101396	5.41	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	108.20%
41) Toluene-d8	7.37	98	213009	4.57	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.40%
43) trans-1,3-Dichloropropene-	7.67	79	30478	4.67	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	93.40%
46) 2-Hexanone-d5	8.15	63	116123	43.56	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	87.12%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	73657	5.04	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.80%
64) 1,2-Dichlorobenzene-d4	11.68	152	77081	5.21	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.20%


Target Compounds					Ovalue
13) Acetone	2.21	43	9547	4.49 ug/L	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV080918\
Data File : VV006966.D
Acq On : 09 Aug 2018 22:41
Operator : SY/MD
Sample : J4399-04
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BC6R4

Quant Time: Aug 10 04:00:49 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080918WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Aug 10 02:34:57 2018
Response via : Initial Calibration

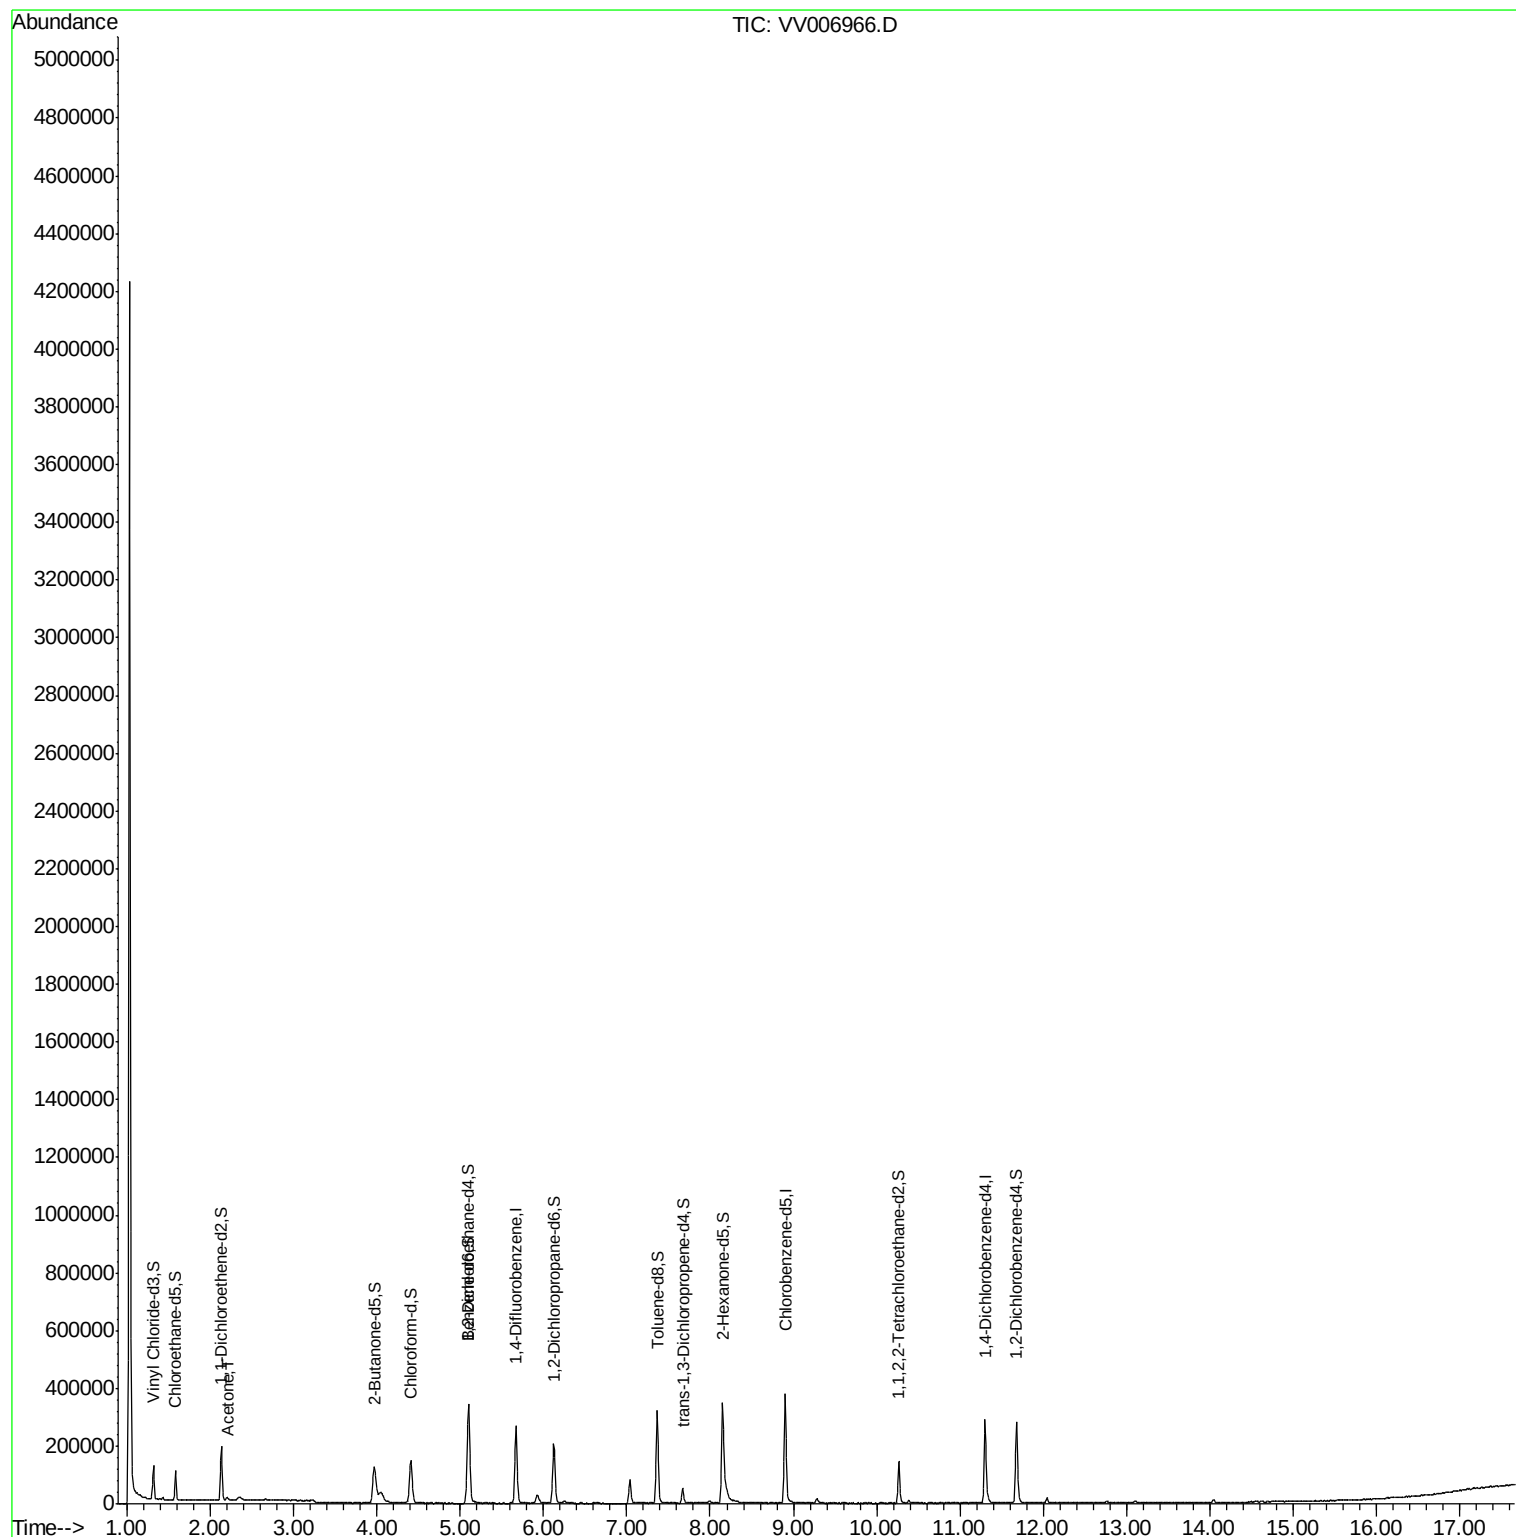

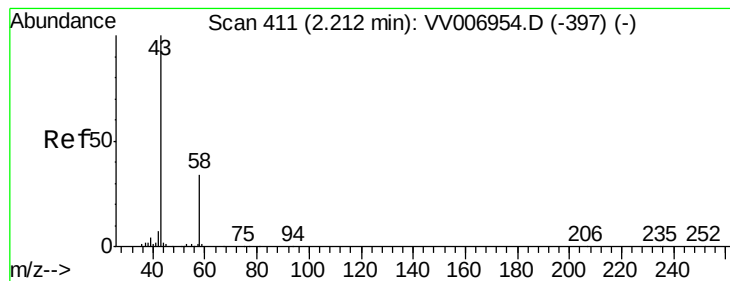

#13

Acetone

Concen: 4.49 ug/L

RT: 2.21 min Scan# 409

Delta R.T. -0.01 min

Lab File: VV006966.D

Acq: 09 Aug 2018 22:41

Instrument :
MSVOA_V
ClientSampleId :
BC6R4

Tot Ion: 43 Resp: 9547

Ion Ratio Lower Upper

43 100

58 43.5 0.0 71.4

