

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV080918\
 Data File : VV006968.D
 Acq On : 09 Aug 2018 23:34
 Operator : SY/MD
 Sample : J4399-08
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BC6R6

Quant Time: Aug 10 04:10:55 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080918WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Aug 10 02:34:57 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	243993	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	228226	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	93115	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	58676	3.73	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	74.60%
7) Chloroethane-d5	1.58	69	66112	4.95	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	99.00%
11) 1,1-Dichloroethene-d2	2.13	63	26281	0.89	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	17.80%#
20) 2-Butanone-d5	3.97	46	265417	58.60	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	117.20%
24) Chloroform-d	4.41	84	156376	4.89	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.80%
26) 1,2-Dichloroethane-d4	5.09	65	83514	5.18	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.60%
32) Benzene-d6	5.10	84	293473	5.01	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.20%
36) 1,2-Dichloropropane-d6	6.12	67	105516	5.27	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	105.40%
41) Toluene-d8	7.37	98	191300	3.83	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	76.60%
43) trans-1,3-Dichloropropene-	7.67	79	32739	4.69	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	93.80%
46) 2-Hexanone-d5	8.15	63	138139	48.44	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.88%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	82947	5.31	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	106.20%
64) 1,2-Dichlorobenzene-d4	11.68	152	81868	5.05	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.00%


Target Compounds					Ovalue
13) Acetone	2.21	43	65950	28.28 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV080918\
Data File : VV006968.D
Acq On : 09 Aug 2018 23:34
Operator : SY/MD
Sample : J4399-08
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BC6R6

Quant Time: Aug 10 04:10:55 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080918WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Aug 10 02:34:57 2018
Response via : Initial Calibration

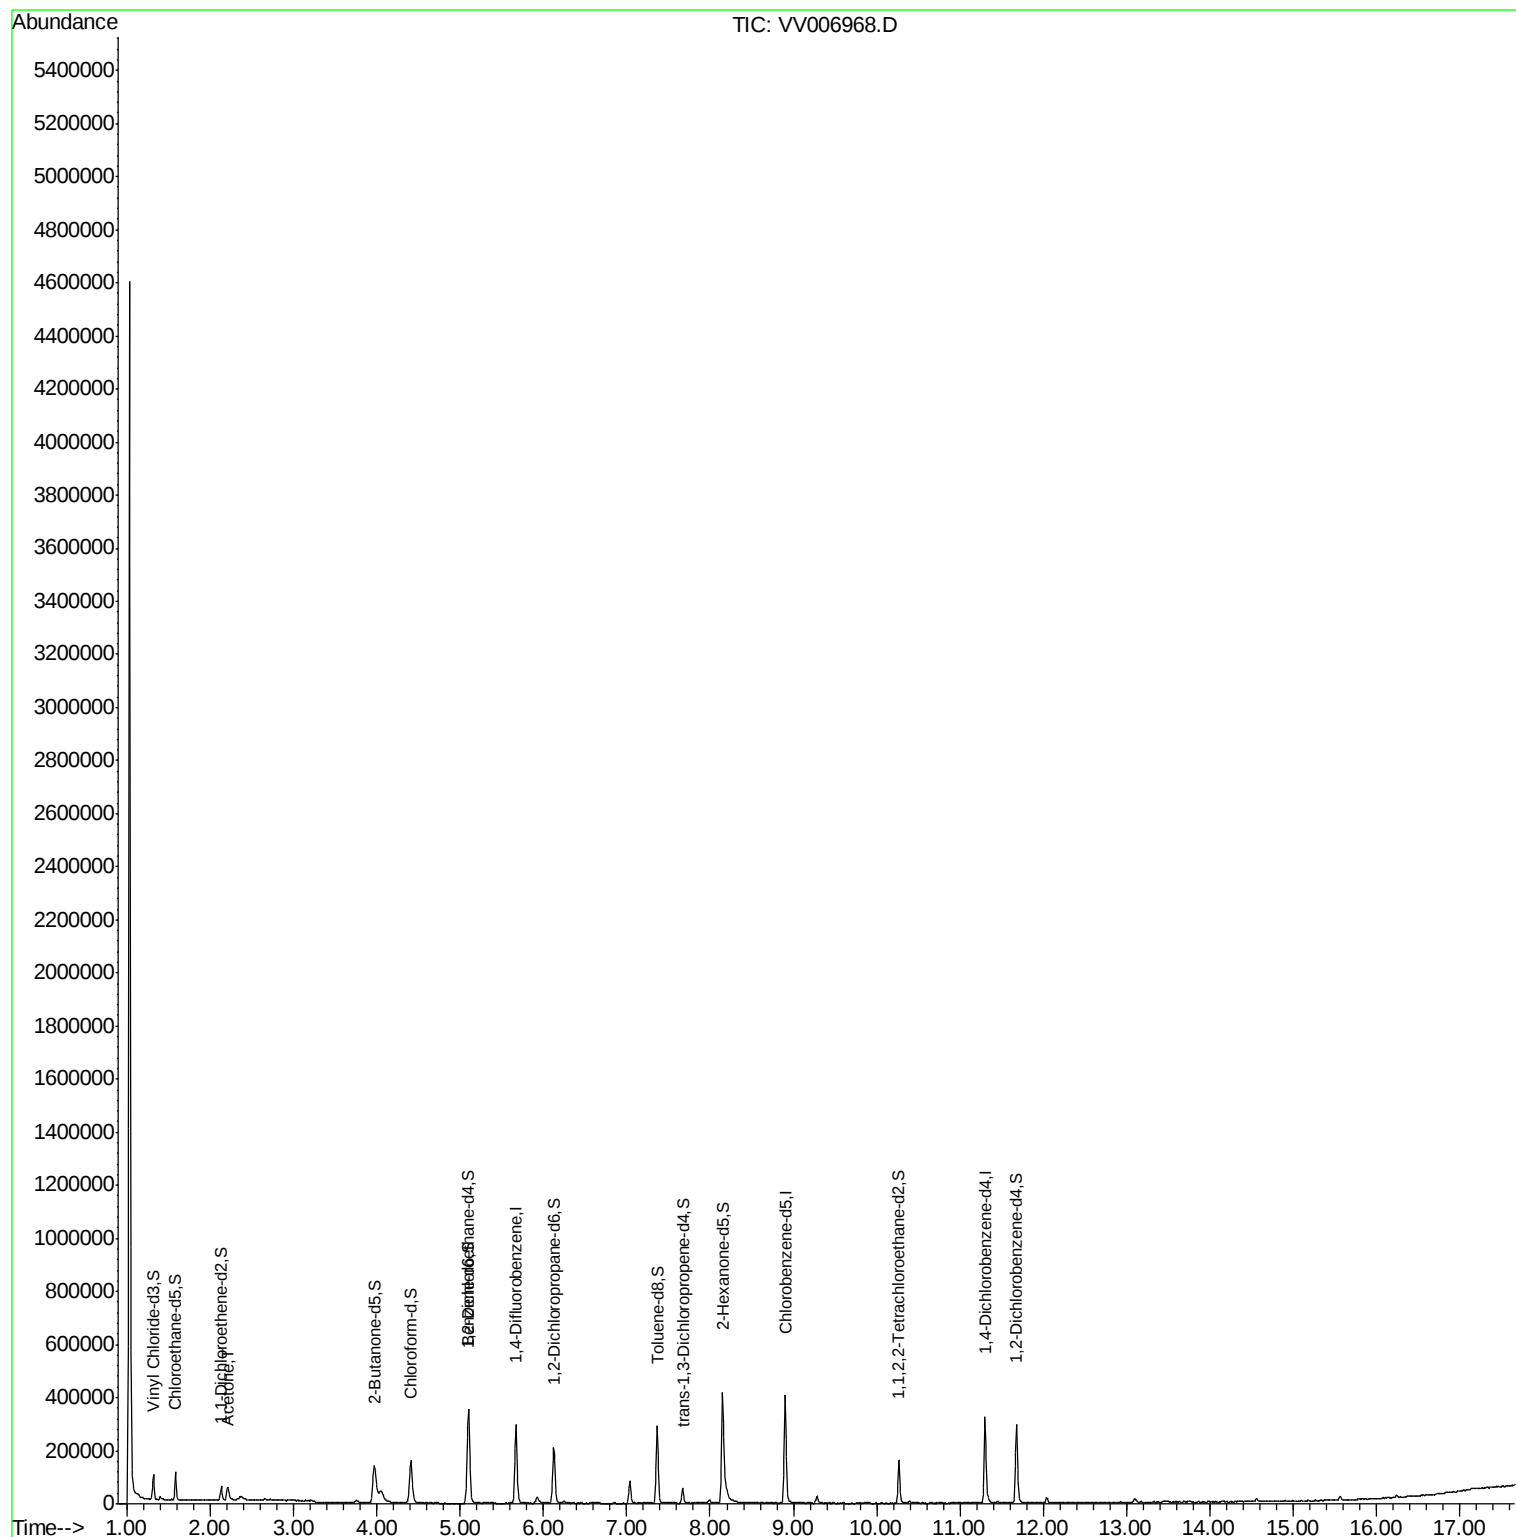

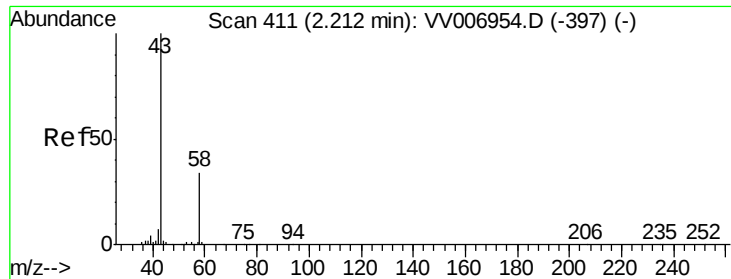

#13

Acetone

Concen: 28.28 ug/L

RT: 2.21 min Scan# 410

Delta R.T. -0.00 min

Lab File: VV006968.D

Acq: 09 Aug 2018 23:34

Instrument :

MSVOA_V

ClientSampleId :

BC6R6

Tot Ion: 43 Resp: 65950

Ion Ratio Lower Upper

43 100

58 35.3 0.0 71.4

