


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV080918\
Data File : VV006946.D
Acq On : 09 Aug 2018 09:50
Operator : SY/MD
Sample : BFB81
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB81

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080918WMA.M
Title : TRACE VOA SOM01.0
Last Update : Fri Aug 10 02:34:57 2018

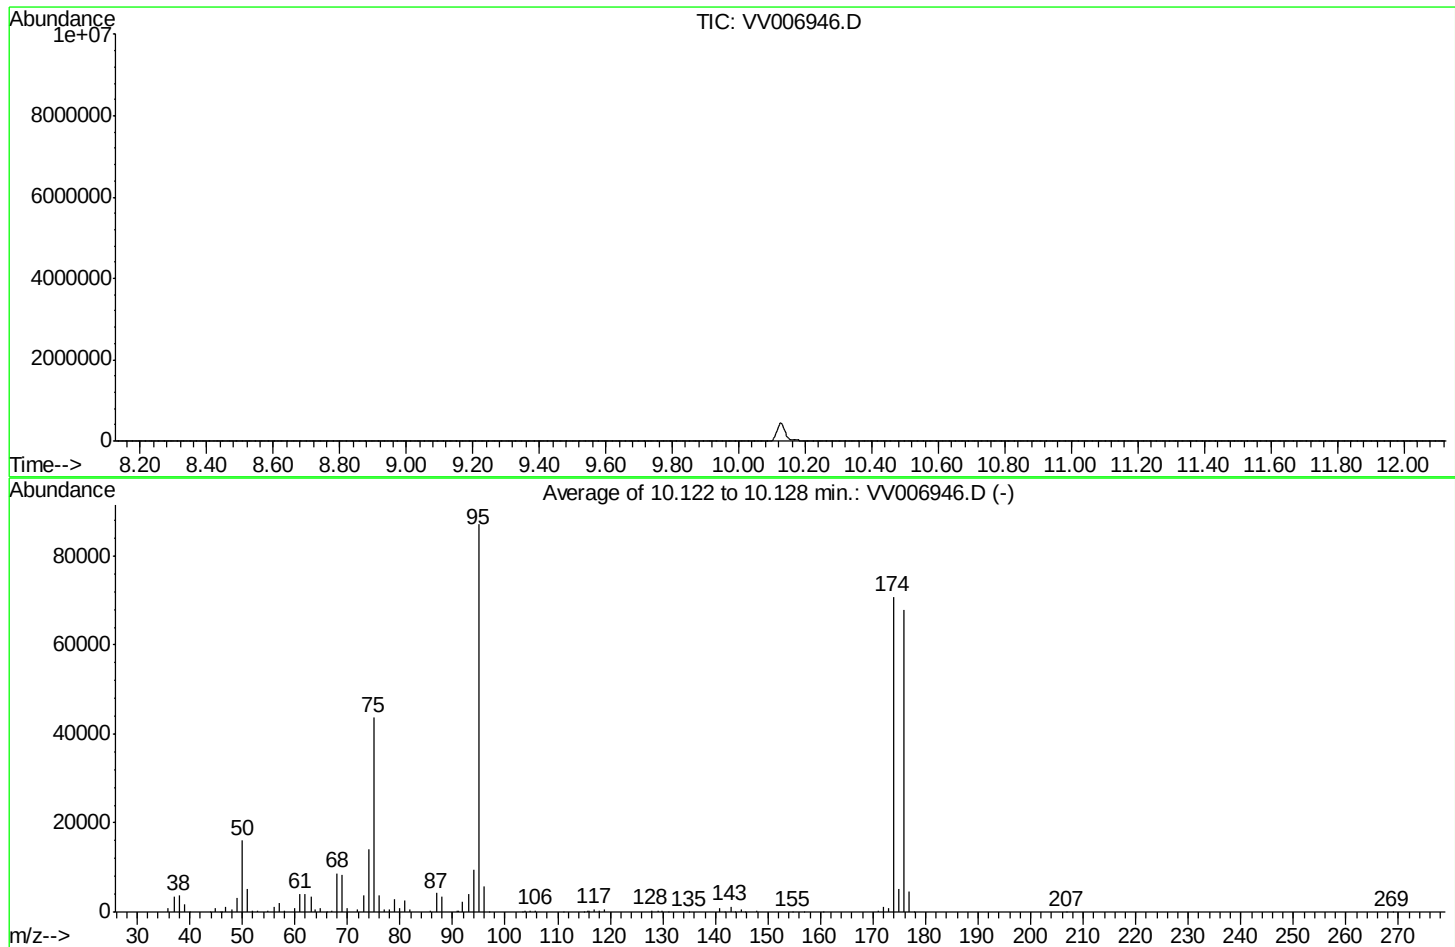

AutoFind: Scans 2871, 2872, 2873; Background Corrected with Scan 2858

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	15981	PASS
75	95	30	80	50.0	43584	PASS
95	95	100	100	100.0	87106	PASS
96	95	5	9	6.5	5669	PASS
173	174	0.00	2	1.1	807	PASS
174	95	50	120	81.3	70792	PASS
175	174	5	9	7.2	5066	PASS
176	174	95	101	95.8	67800	PASS
177	176	5	9	6.7	4520	PASS

Scan 2858 (10.080 min): VV006946.D
BFB81

m/z	Abundance
39.90	536.0
41.10	104.0
43.00	134.0
44.00	1354.0
77.00	180.0
206.90	180.0

Instrument :
MSVOA_V
ClientSampleId :
BFB81

m/z	Abundance
35.90	760.0
37.00	3150.0
38.00	3728.0
39.00	1684.0
40.00	595.0
40.90	107.0
43.10	112.0
43.90	1428.0
44.90	688.0
45.80	102.0
46.20	140.0
46.90	890.0
48.10	567.0
48.90	2864.0
50.00	15494.0
51.00	4976.0
51.90	210.0
53.00	194.0
54.90	313.0
56.00	956.0
57.00	1915.0
57.90	203.0
60.00	747.0
61.00	4188.0
62.00	3929.0
63.00	3384.0
64.00	675.0
64.90	829.0
65.90	130.0
66.90	353.0
68.00	7958.0
69.00	8283.0
70.00	693.0
71.80	446.0
73.00	3344.0
74.00	13657.0
75.00	41704.0
76.00	3653.0
77.00	852.0
77.90	505.0
78.90	2808.0
80.00	806.0
80.90	2388.0
81.90	516.0
85.80	281.0
86.90	3931.0
88.00	3118.0
90.70	158.0
91.10	144.0
91.90	2374.0
93.00	3737.0
94.00	8973.0
95.00	82736.0
96.00	5326.0
96.90	124.0
103.80	352.0
104.70	154.0
105.80	363.0
111.00	108.0
115.00	151.0
115.80	220.0
116.10	216.0
116.90	683.0
118.00	255.0
118.90	569.0
127.90	368.0
129.00	141.0
129.80	261.0
140.90	742.0
141.90	144.0
142.90	1168.0
143.80	118.0
144.90	572.0
145.90	108.0
147.80	145.0
154.70	150.0
160.60	134.0
170.90	162.0
171.90	1080.0
173.00	814.0
173.90	65376.0
174.90	4778.0
175.90	62208.0
176.90	4299.0
177.90	137.0
207.10	367.0

Instrument :
MSVOA_V
ClientSampleId :
BFB81

m/z	Abundance
35.90	788.0
37.00	3476.0
38.00	3869.0
39.00	1829.0
39.90	638.0
40.90	105.0
43.00	104.0
43.90	1437.0
44.90	749.0
45.80	142.0
46.20	153.0
46.90	1126.0
48.10	567.0
49.00	3174.0
50.00	16600.0
51.00	5353.0
52.00	231.0
52.90	227.0
54.90	368.0
56.00	1067.0
57.00	2115.0
57.90	189.0
60.00	901.0
61.00	4298.0
62.00	4140.0
63.00	3634.0
64.00	700.0
64.90	916.0
65.90	148.0
66.90	335.0
68.00	8983.0
69.00	8581.0
70.00	764.0
71.90	514.0
73.00	3693.0
74.00	14523.0
75.00	44856.0
76.00	3818.0
76.90	858.0
78.00	465.0
78.90	2941.0
80.00	847.0
80.90	2741.0
81.90	549.0
85.80	325.0
86.90	4379.0
87.90	3456.0
90.70	199.0
91.10	191.0
91.90	2505.0
93.00	4020.0
94.00	9739.0
95.00	89584.0
96.00	5827.0
96.90	113.0
103.80	403.0
104.70	196.0
105.80	421.0
111.00	116.0
115.00	155.0
115.70	289.0
117.00	734.0
118.00	289.0
118.90	613.0
127.90	337.0
129.00	243.0
129.90	378.0
131.00	147.0
135.00	121.0
140.90	840.0
141.80	141.0
142.90	1351.0
143.80	110.0
144.90	610.0
145.70	137.0
147.80	194.0
154.70	128.0
156.90	108.0
171.00	188.0
171.90	1242.0
173.00	821.0
173.90	73000.0
175.00	5222.0
175.90	69912.0
176.90	4663.0
206.90	311.0
268.90	162.0

Instrument :
MSVOA_V
ClientSampleId :
BFB81

m/z	Abundance
35.90	727.0
37.00	3465.0
38.00	3594.0
39.00	1800.0
39.90	658.0
42.90	106.0
43.90	1476.0
44.90	867.0
45.80	175.0
46.10	149.0
46.90	1246.0
48.10	538.0
49.00	3407.0
50.00	15849.0
51.00	5103.0
52.00	200.0
52.90	222.0
54.90	330.0
55.90	1070.0
57.00	2283.0
57.90	161.0
60.00	962.0
61.00	3947.0
62.00	4214.0
63.00	3657.0
63.90	672.0
64.90	899.0
66.00	156.0
66.90	272.0
68.00	9018.0
69.00	8260.0
70.00	746.0
71.90	532.0
73.00	3807.0
74.00	14358.0
75.00	44192.0
76.00	3731.0
76.90	771.0
78.10	362.0
78.90	2756.0
79.90	836.0
80.90	2808.0
81.90	587.0
85.80	298.0
86.90	4531.0
87.90	3724.0
90.80	223.0
91.00	228.0
92.00	2272.0
93.00	3926.0
94.00	9876.0
95.00	89000.0
96.00	5856.0
103.20	101.0
103.80	376.0
104.70	160.0
105.80	393.0
114.90	146.0
115.80	294.0
116.00	312.0
117.00	666.0
118.00	297.0
118.90	625.0
127.80	332.0
129.00	280.0
129.90	394.0
130.90	142.0
140.80	817.0
141.80	115.0
142.90	1295.0
144.90	527.0
145.70	153.0
147.80	233.0
156.90	163.0
170.90	187.0
172.00	1207.0
172.90	788.0
173.90	74000.0
175.00	5199.0
175.90	71280.0
176.90	4599.0
206.90	276.0
268.90	157.0

Instrument :
MSVOA_V
ClientSampleId :
BFB81