

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV080919\
 Data File : VV012153.D
 Acq On : 09 Aug 2019 15:07
 Operator : SY/MD
 Sample : K4214-04
 Misc : 25mL/MSVOA V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Quant Time: Aug 10 03:25:34 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080819WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Aug 10 02:29:42 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	154078	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	144775	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	76045	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	29990	4.57	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	91.40%
7) Chloroethane-d5	1.58	69	22927	4.77	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	95.40%
11) 1,1-Dichloroethene-d2	2.13	63	46153	3.48	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	69.60%
20) 2-Butanone-d5	3.95	46	76240	45.05	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	90.10%
24) Chloroform-d	4.40	84	83163	4.37	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.40%
26) 1,2-Dichloroethane-d4	5.08	65	42577	4.30	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.00%
32) Benzene-d6	5.09	84	162577	4.57	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.40%
36) 1,2-Dichloropropane-d6	6.11	67	44039	4.69	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.80%
41) Toluene-d8	7.36	98	156405	4.34	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.80%
43) trans-1,3-Dichloropropene-	7.66	79	19528	3.98	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	79.60%
46) 2-Hexanone-d5	8.13	63	66351	42.49	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	84.98%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	33102	4.28	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	85.60%
64) 1,2-Dichlorobenzene-d4	11.67	152	66746	4.72	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	94.40%


Target Compounds					Ovalue
16) Methylene chloride	2.53	84	1593	0.244 ug/L	# 88




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV080919\
Data File : VV012153.D
Acq On : 09 Aug 2019 15:07
Operator : SY/MD
Sample : K4214-04
Misc : 25mL/MSVOA V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Time: Aug 10 03:25:34 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080819WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Aug 10 02:29:42 2019
Response via : Initial Calibration

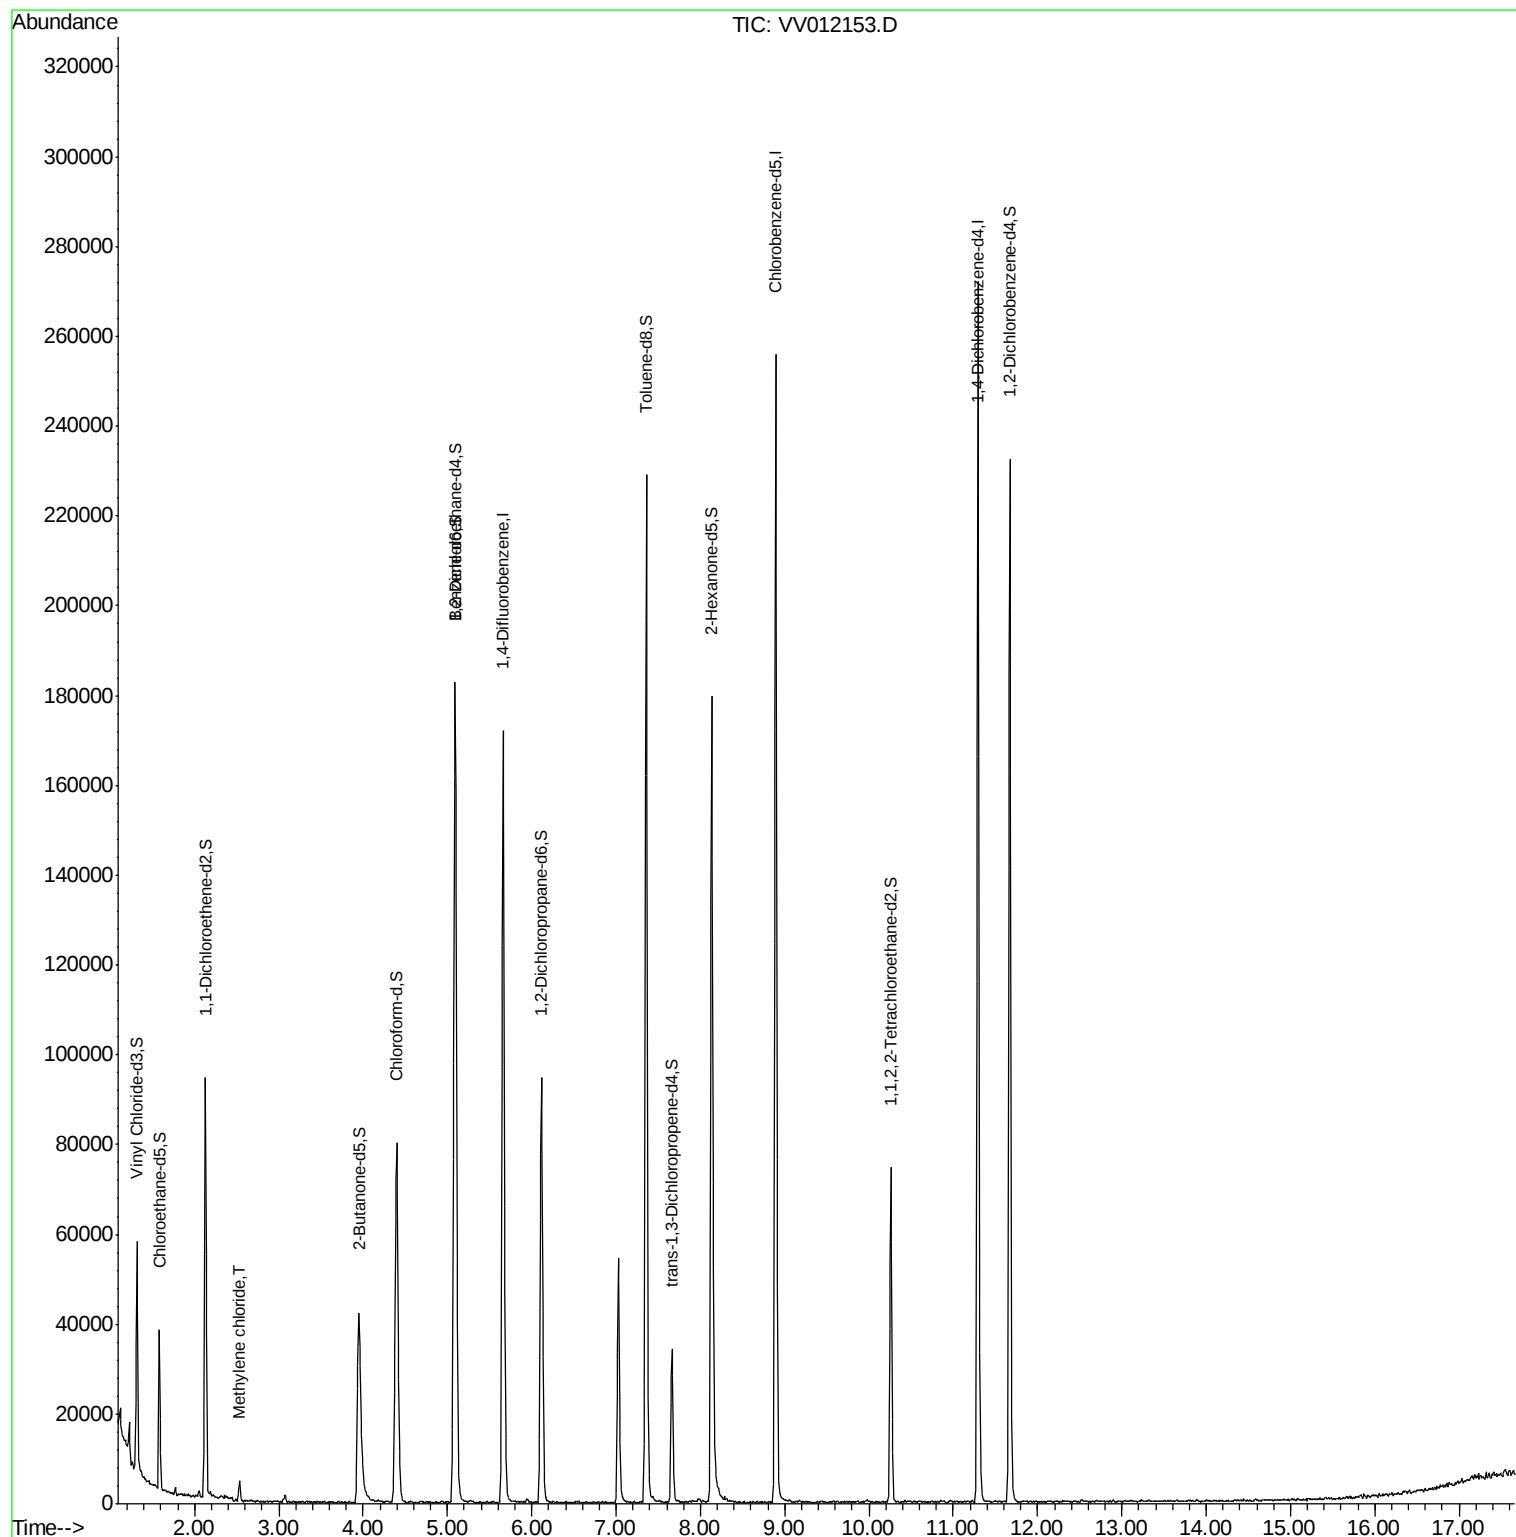

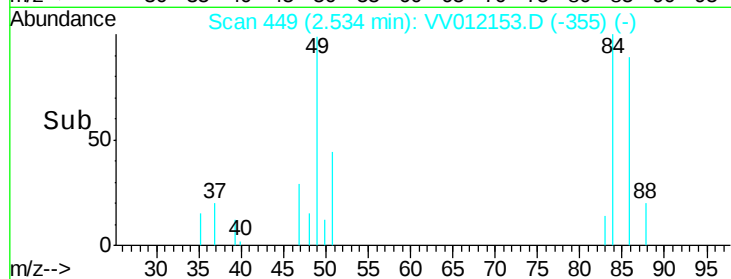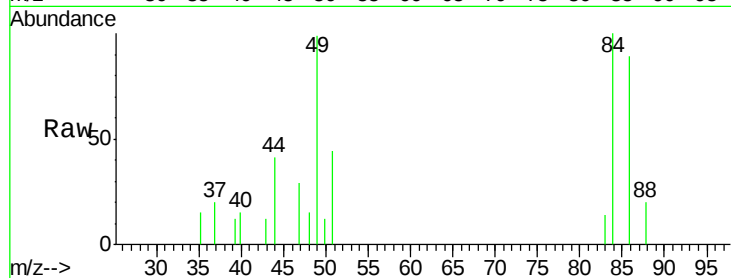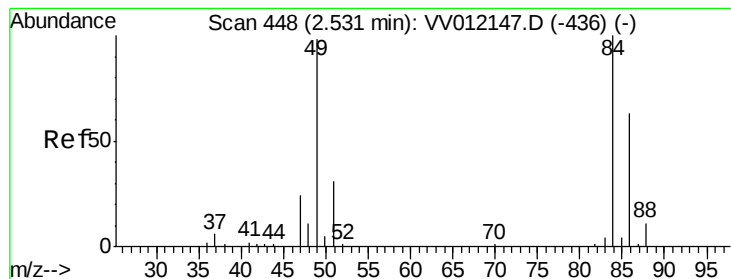

#16

Methylene chloride

Concen: 0.244 ug/L

RT: 2.53 min Scan# 449

Delta R.T. 0.00 min

Lab File: VV012153.D

Acq: 09 Aug 2019 15:07

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Tot Ion:	84	Resp:	1593
Ion	Ratio	Lower	Upper
84	100		
86	88.5	45.4	84.2#
49	98.5	69.2	128.4

