


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV080919\
Data File : VV012146.D
Acq On : 09 Aug 2019 09:08
Operator : SY/MD
Sample : BFB45
Misc : 25mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB45

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080819WMA.M
Title : TRACE VOA SOM01.0
Last Update : Mon Aug 12 14:50:23 2019

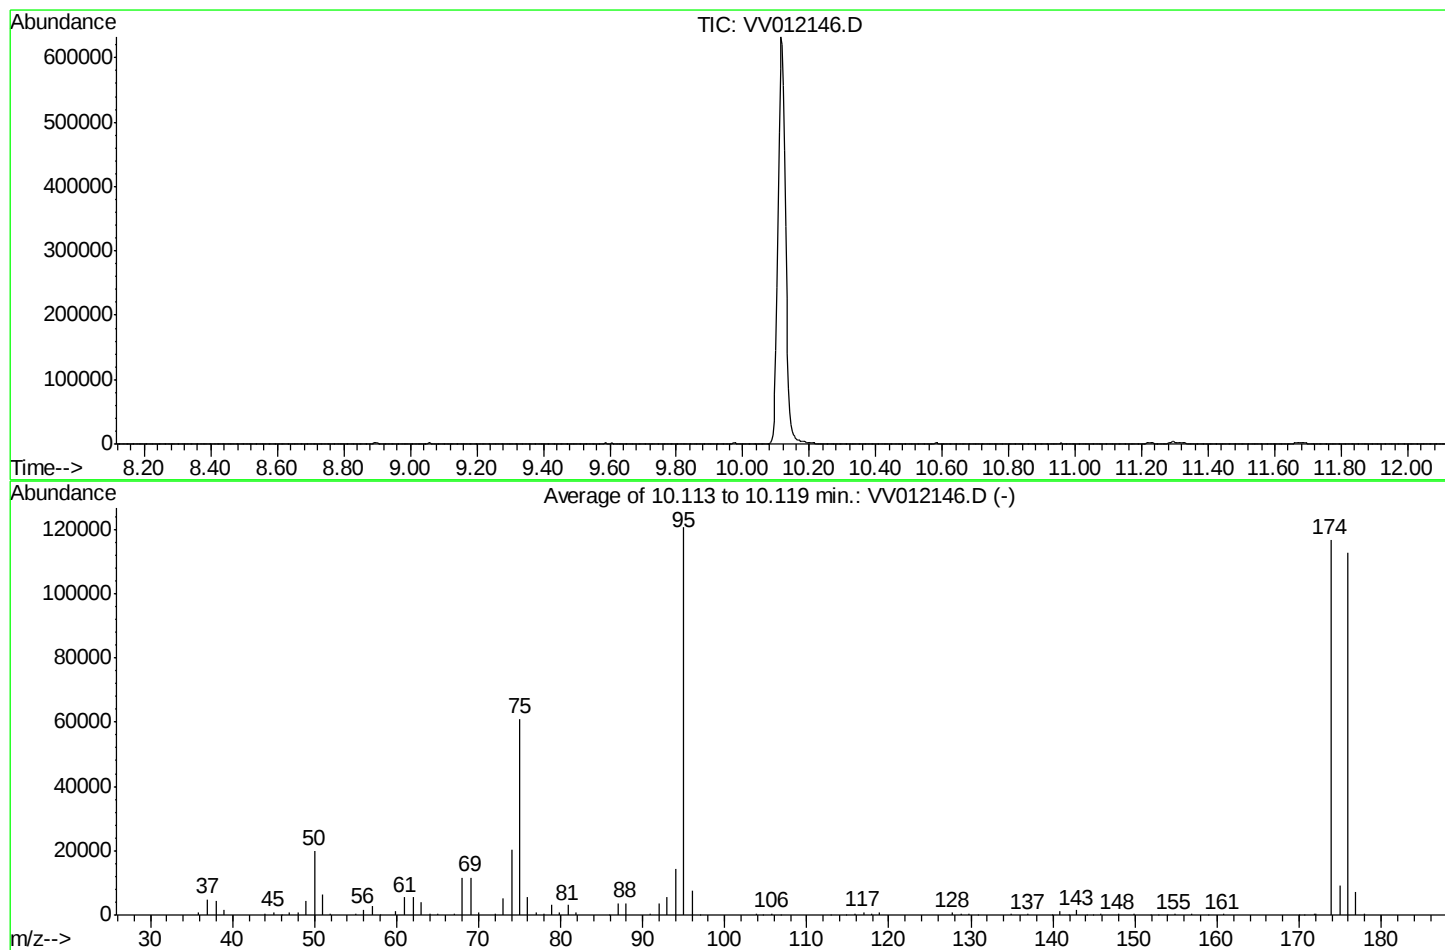

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	20101	PASS
75	95	30	80	50.6	61034	PASS
95	95	100	100	100.0	120589	PASS
96	95	5	9	6.4	7763	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	96.7	116664	PASS
175	174	5	9	7.9	9203	PASS
176	174	95	101	96.5	112602	PASS
177	176	5	9	6.3	7145	PASS

m/z	Abundance
35.90	832.0
36.90	4574.0
38.00	4397.0
39.00	1575.0
39.90	166.0
44.00	679.0
45.00	716.0
46.90	873.0
48.00	824.0
49.00	4271.0
50.00	19632.0
51.00	6162.0
51.90	315.0
54.90	307.0
55.90	1595.0
57.00	2854.0
58.00	112.0
59.90	1096.0
61.00	5384.0
62.00	5339.0
63.00	3865.0
64.00	388.0
65.00	424.0
67.00	369.0
68.00	11084.0
69.00	11418.0
70.10	972.0
72.00	562.0
73.00	4959.0
74.00	19536.0
75.00	59304.0
76.00	5238.0
77.00	645.0
77.90	320.0
78.90	3105.0
79.90	1001.0
80.90	3113.0
81.90	636.0
85.90	119.0
87.00	3558.0
87.90	3684.0
91.00	376.0
92.00	3378.0
93.00	5212.0
94.00	14029.0
95.00	115696.0
96.00	7548.0
97.00	229.0
103.90	469.0
104.70	177.0
105.80	543.0
106.90	145.0
113.00	105.0
114.80	176.0
115.80	374.0
116.90	763.0
117.90	518.0
118.90	507.0
127.80	575.0
128.80	199.0
129.80	479.0
130.90	187.0
134.90	224.0
137.00	264.0
139.90	124.0
140.90	1274.0
142.90	1462.0
144.80	181.0
145.90	226.0
148.00	281.0
149.90	205.0
152.80	195.0
153.90	121.0
154.90	384.0
156.90	245.0
158.80	144.0
160.70	177.0
170.60	103.0
171.80	691.0
173.90	108792.0
175.00	8603.0
175.90	104768.0
176.90	6732.0
178.00	258.0

Instrument :
MSVOA_V
ClientSampleId :
BFB45

m/z	Abundance
35.90	801.0
36.90	4958.0
38.00	4563.0
38.90	1714.0
39.90	110.0
43.90	751.0
45.00	849.0
45.90	122.0
46.90	914.0
47.90	904.0
49.00	4675.0
50.00	20672.0
51.00	6483.0
51.90	333.0
54.90	354.0
55.90	1753.0
57.00	2992.0
58.00	137.0
59.90	1144.0
61.00	5681.0
62.00	5586.0
63.00	3870.0
64.00	398.0
65.00	340.0
67.00	320.0
68.00	12171.0
69.00	12063.0
70.10	1056.0
72.00	562.0
73.00	5162.0
74.00	20936.0
75.00	63064.0
76.00	5666.0
77.00	672.0
77.90	371.0
78.90	3327.0
79.90	1033.0
80.90	3240.0
81.90	660.0
85.80	137.0
87.00	3768.0
87.90	3891.0
91.00	526.0
92.00	3639.0
93.00	5577.0
94.00	14997.0
95.00	124440.0
96.00	7983.0
97.00	207.0
103.90	522.0
104.70	179.0
105.80	581.0
106.90	159.0
112.90	107.0
114.70	168.0
115.80	430.0
116.90	845.0
117.80	574.0
118.80	627.0
127.80	672.0
128.80	218.0
129.80	529.0
130.90	161.0
135.00	247.0
137.00	286.0
140.00	169.0
140.90	1357.0
142.00	142.0
142.90	1518.0
144.10	113.0
144.90	179.0
145.80	245.0
147.90	306.0
149.90	233.0
151.90	106.0
152.80	221.0
154.00	146.0
154.80	362.0
156.90	295.0
158.80	193.0
160.80	239.0
170.00	111.0
170.70	103.0
171.80	697.0
173.90	120680.0
175.00	9528.0
175.90	116080.0
176.90	7339.0
178.00	266.0

Instrument :
MSVOA_V
ClientSampleId :
BFB45

m/z	Abundance
35.90	730.0
37.00	4812.0
38.00	4145.0
38.90	1814.0
43.90	777.0
45.00	862.0
45.90	129.0
46.90	884.0
48.00	825.0
49.00	4570.0
50.00	20000.0
51.00	6194.0
51.90	264.0
55.00	320.0
55.90	1646.0
57.00	2977.0
58.00	107.0
59.90	1078.0
61.00	5353.0
62.00	5313.0
63.00	3719.0
64.00	389.0
64.90	303.0
67.00	261.0
68.00	11809.0
69.00	11673.0
70.00	979.0
72.00	556.0
73.00	5012.0
74.00	20384.0
75.00	60736.0
76.00	5441.0
77.00	583.0
78.00	385.0
78.90	3128.0
79.90	946.0
80.90	3076.0
81.90	673.0
85.80	126.0
87.00	3660.0
87.90	3649.0
90.90	565.0
92.00	3507.0
93.00	5497.0
94.00	14455.0
95.00	121632.0
96.00	7758.0
96.90	192.0
103.90	498.0
104.70	160.0
105.80	537.0
106.80	153.0
112.80	115.0
114.90	170.0
115.80	432.0
116.90	860.0
117.80	513.0
118.80	708.0
127.80	643.0
128.90	245.0
129.80	564.0
130.90	139.0
135.00	251.0
136.90	262.0
140.00	184.0
140.90	1425.0
141.90	168.0
142.90	1479.0
144.10	123.0
144.90	161.0
145.80	202.0
147.90	334.0
149.80	218.0
151.90	144.0
152.80	163.0
154.00	159.0
154.80	378.0
156.90	335.0
158.90	257.0
160.80	241.0
170.00	104.0
172.00	668.0
173.90	120520.0
174.90	9478.0
175.90	116960.0
176.90	7366.0
177.90	213.0

Instrument :
MSVOA_V
ClientSampleId :
BFB45

Scan 2794 (10.074 min): VV012146.D
BFB45

m/z	Abundance
40.00	147.0
43.90	162.0

Instrument :
MSVOA_V
ClientSampleId :
BFB45