


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080921\
 Data File : VV021756.D
 Acq On : 09 Aug 2021 09:28
 Operator : SY/MD
 Sample : BFB214
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB214

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080221WMA.M
 Title : VOC Analysis
 Last Update : Tue Aug 10 01:21:22 2021

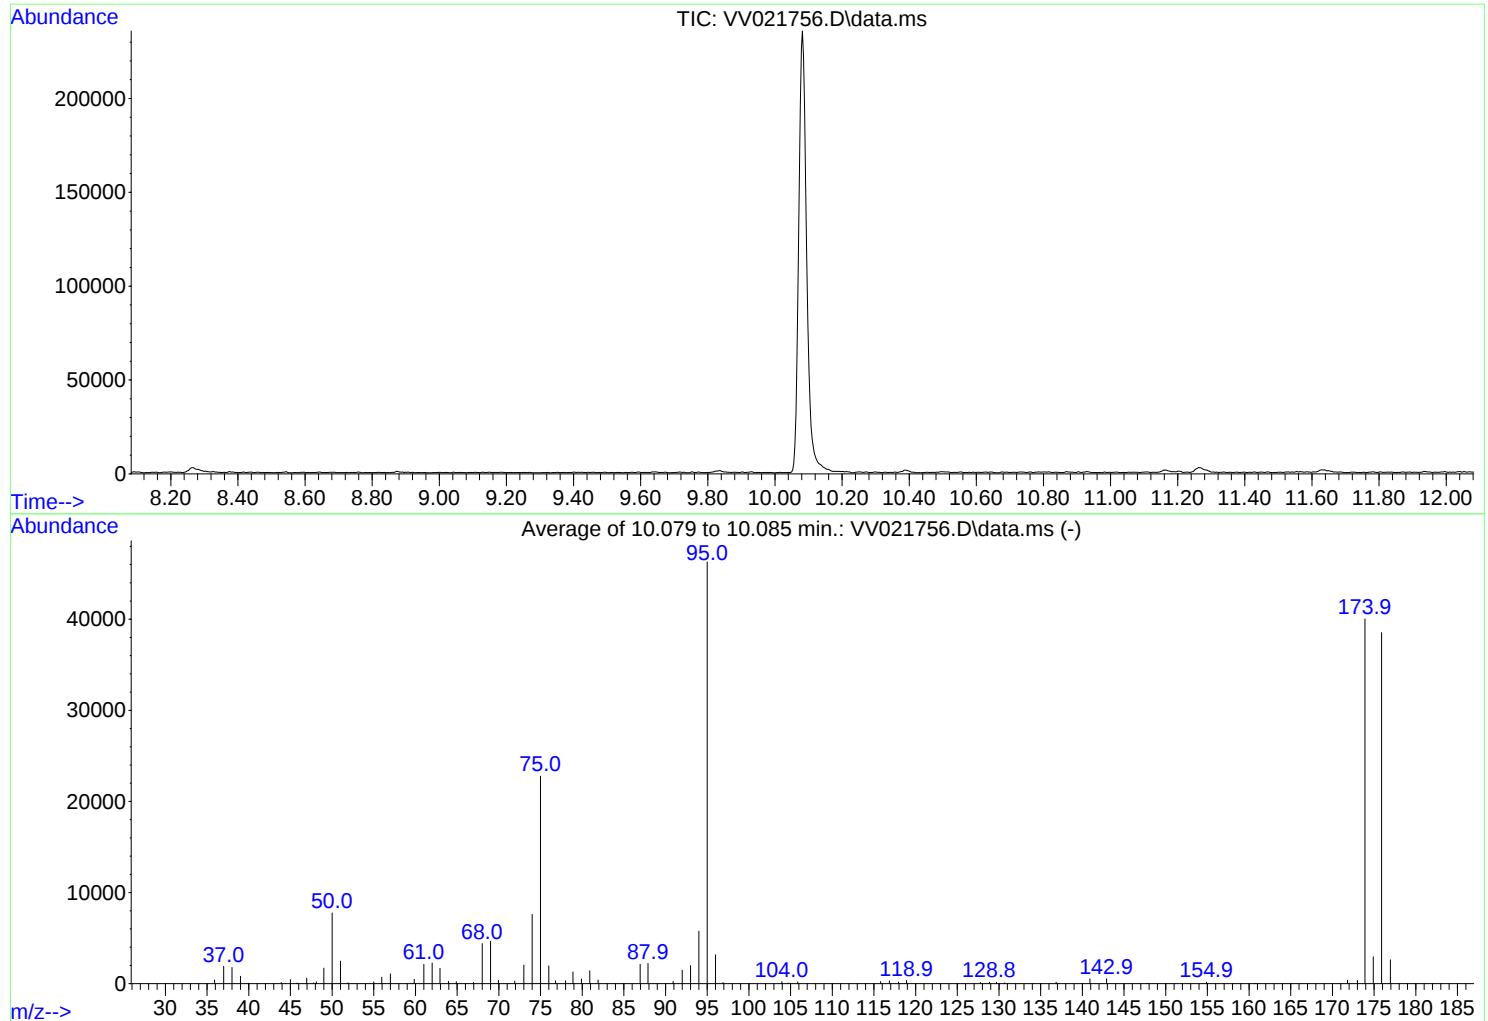

AutoFind: Scans 2811, 2812, 2813; Background Corrected with Scan 2800

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	7763	PASS
75	95	30	80	49.2	22784	PASS
95	95	100	100	100.0	46299	PASS
96	95	5	9	6.8	3162	PASS
173	174	0.00	2	0.9	345	PASS
174	95	50	120	86.5	40043	PASS
175	174	5	9	7.4	2955	PASS
176	174	95	105	96.2	38528	PASS
177	176	5	10	6.8	2620	PASS

Scan 2800 (10.043 min): VV021756.D\data.ms
BFB214

m/z	Abundance
39.90	233.0
43.90	485.0

Instrument :
MSVOA_V
ClientSampleId :
BFB214

m/z	Abundance
35.90	369.0
37.00	1778.0
38.00	1751.0
39.00	752.0
40.00	293.0
43.90	603.0
45.00	417.0
47.00	620.0
48.10	370.0
49.00	1632.0
50.00	7417.0
51.00	2441.0
51.90	144.0
55.00	197.0
56.00	669.0
57.00	1034.0
59.90	373.0
61.00	1829.0
62.00	2148.0
62.90	1631.0
64.00	248.0
64.90	226.0
67.00	125.0
68.00	4240.0
69.00	4359.0
70.00	314.0
71.90	274.0
73.00	1896.0
74.00	7319.0
75.00	22320.0
76.00	1851.0
76.80	286.0
78.00	277.0
78.90	1251.0
79.90	458.0
80.90	1359.0
81.90	411.0
86.90	1950.0
87.90	2252.0
91.00	237.0
92.00	1443.0
93.00	1846.0
94.00	5544.0
95.00	44896.0
96.00	2932.0
96.90	101.0
103.90	231.0
104.70	102.0
105.90	209.0
115.80	212.0
116.90	288.0
117.90	165.0
118.90	321.0
127.70	125.0
128.90	139.0
129.70	144.0
136.80	132.0
140.90	512.0
142.90	502.0
147.90	124.0
154.90	149.0
160.70	110.0
171.80	325.0
173.00	351.0
173.90	40032.0
174.90	2777.0
175.90	38272.0
177.00	2401.0

Instrument :
MSVOA_V
ClientSampleId :
BFB214

m/z	Abundance
35.90	410.0
37.00	1953.0
38.00	1832.0
39.00	812.0
40.00	296.0
43.90	617.0
45.00	457.0
45.80	106.0
46.90	622.0
48.10	294.0
49.00	1726.0
50.00	7992.0
51.00	2551.0
51.90	125.0
55.00	199.0
56.00	709.0
57.00	1117.0
59.80	475.0
61.00	2178.0
62.00	2405.0
62.90	1733.0
63.90	264.0
64.90	207.0
67.00	130.0
68.00	4542.0
69.00	4808.0
69.90	380.0
71.90	284.0
73.00	2133.0
74.00	7876.0
75.00	23416.0
76.00	2020.0
76.80	349.0
78.00	317.0
78.90	1310.0
79.90	517.0
80.90	1457.0
81.90	413.0
86.90	2195.0
87.90	2342.0
90.90	238.0
92.00	1551.0
93.00	2044.0
94.00	5948.0
95.00	47608.0
96.00	3257.0
96.90	133.0
103.90	245.0
104.70	103.0
105.90	192.0
115.80	239.0
116.90	307.0
118.00	185.0
118.90	366.0
127.70	144.0
128.90	155.0
129.70	159.0
130.70	133.0
136.90	169.0
140.90	543.0
142.90	551.0
147.70	108.0
154.90	156.0
171.80	417.0
173.00	341.0
173.90	41432.0
174.90	3069.0
175.90	39848.0
176.90	2719.0

Instrument :
MSVOA_V
ClientSampleId :
BFB214

m/z	Abundance
35.90	413.0
37.00	1945.0
38.00	1726.0
39.00	836.0
40.00	276.0
43.90	612.0
45.00	444.0
45.80	114.0
46.90	565.0
47.80	258.0
49.00	1729.0
50.00	7879.0
51.00	2462.0
55.00	183.0
55.90	724.0
57.00	1081.0
59.80	556.0
61.00	2329.0
62.00	2265.0
63.00	1672.0
63.90	221.0
64.90	189.0
66.90	132.0
68.00	4395.0
69.00	4783.0
69.90	429.0
71.90	291.0
73.00	2090.0
74.00	7622.0
75.00	22616.0
76.00	1965.0
76.80	333.0
78.00	353.0
78.90	1275.0
79.90	568.0
80.90	1429.0
81.90	383.0
87.00	2243.0
87.90	2035.0
90.80	252.0
92.00	1411.0
93.00	2086.0
94.00	5805.0
95.00	46392.0
96.00	3297.0
96.90	135.0
104.00	230.0
105.80	167.0
115.80	251.0
116.80	297.0
118.00	162.0
118.90	365.0
127.80	163.0
128.80	161.0
129.70	149.0
130.70	159.0
136.90	179.0
140.90	514.0
142.90	543.0
154.90	174.0
171.80	416.0
173.00	344.0
173.90	38664.0
174.90	3019.0
175.90	37464.0
176.90	2740.0

Instrument :
MSVOA_V
ClientSampleId :
BFB214