

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081018\
 Data File : VV006983.D
 Acq On : 10 Aug 2018 14:50
 Operator : SY/MD
 Sample : J4422-06
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AC2

Quant Time: Aug 13 11:29:11 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080918WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Aug 10 23:13:31 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	265469	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	256790	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	103497	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	70789	4.13	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	82.60%
7) Chloroethane-d5	1.58	69	65640	4.52	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.40%
11) 1,1-Dichloroethene-d2	2.13	63	97658	3.04	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	60.80%
20) 2-Butanone-d5	3.97	46	232957	47.27	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	94.54%
24) Chloroform-d	4.40	84	160235	4.61	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.20%
26) 1,2-Dichloroethane-d4	5.09	65	83079	4.73	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.60%
32) Benzene-d6	5.10	84	298121	4.52	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.40%
36) 1,2-Dichloropropane-d6	6.12	67	105706	4.69	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.80%
41) Toluene-d8	7.36	98	219888	3.92	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	78.40%
43) trans-1,3-Dichloropropene-	7.67	79	32092	4.09	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.80%
46) 2-Hexanone-d5	8.15	63	113512	35.38	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	70.76%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	75618	4.30	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	86.00%
64) 1,2-Dichlorobenzene-d4	11.68	152	81752	4.54	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	90.80%


Target Compounds					Ovalue
13) Acetone	2.22	43	7322	2.89 ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV081018\
Data File : VV006983.D
Acq On : 10 Aug 2018 14:50
Operator : SY/MD
Sample : J4422-06
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AC2

Quant Time: Aug 13 11:29:11 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080918WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Aug 10 23:13:31 2018
Response via : Initial Calibration

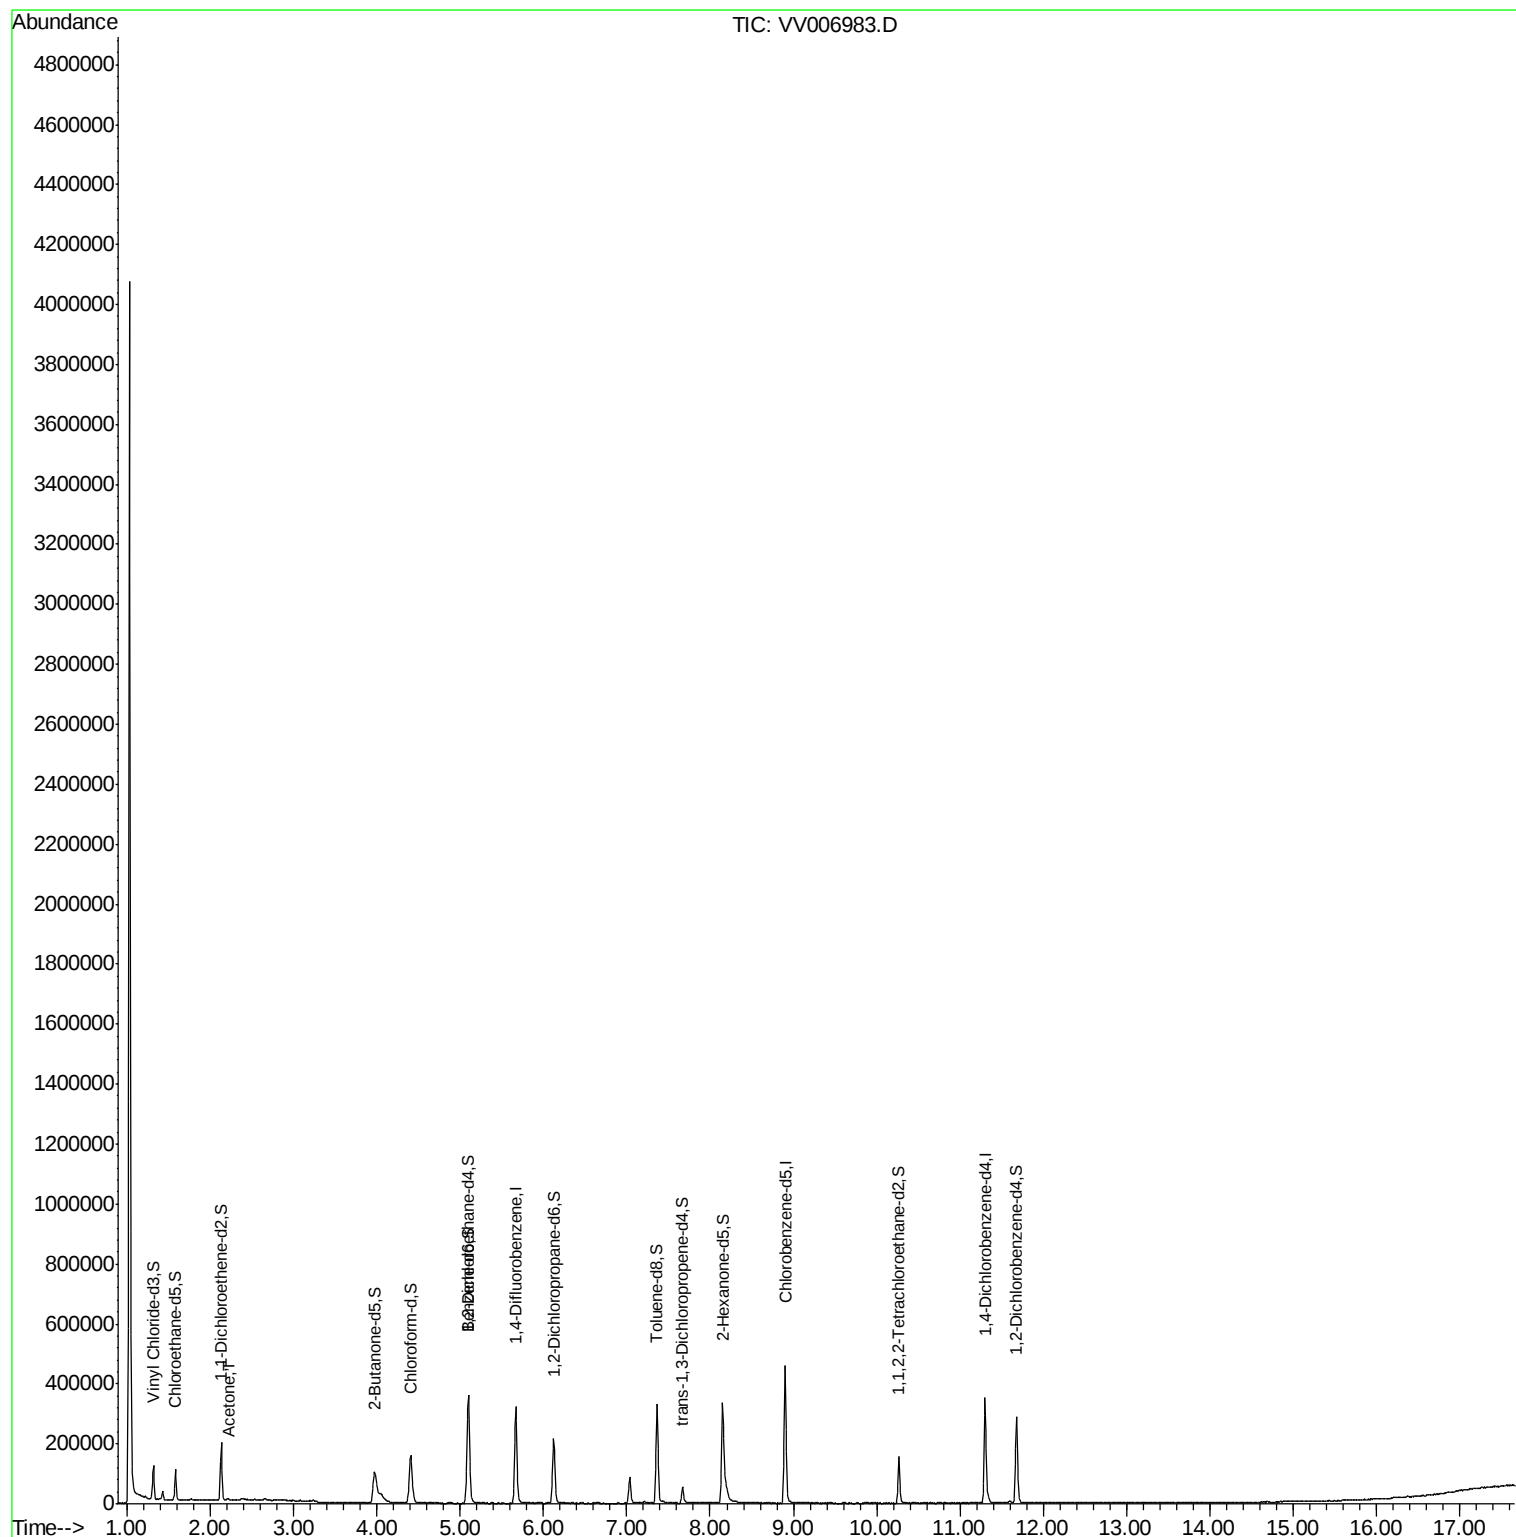

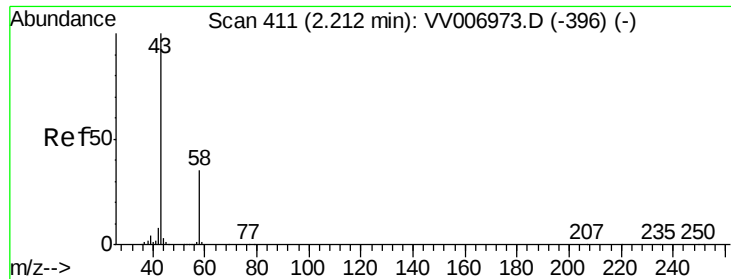

#13

Acetone

Concen: 2.89 ug/L

RT: 2.22 min Scan# 413

Delta R.T. 0.01 min

Lab File: VV006983.D

Acq: 10 Aug 2018 14:50

Instrument :
MSVOA_V
ClientSampleId :
C0AC2

Tot Ion: 43 Resp: 7322

Ion Ratio Lower Upper

43 100

58 35.8 0.0 71.4

