


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081018\
Data File : VV006972.D
Acq On : 10 Aug 2018 08:57
Operator : SY/MD
Sample : BFB82
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB82

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080918WMA.M
Title : TRACE VOA SOM01.0
Last Update : Sat Aug 11 00:19:35 2018

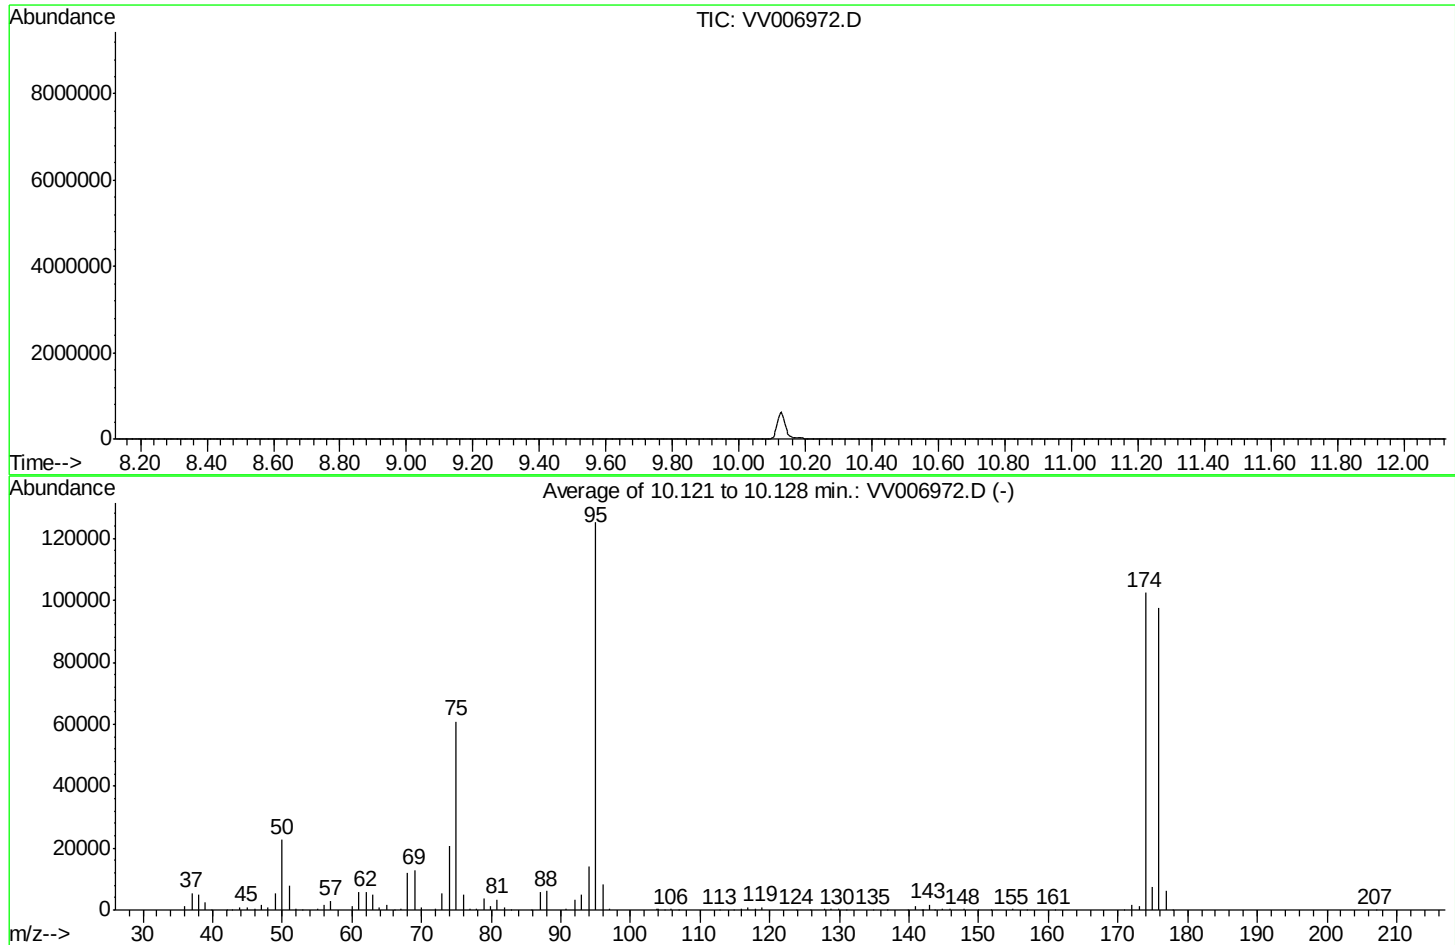

AutoFind: Scans 2871, 2872, 2873; Background Corrected with Scan 2858

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	22685	PASS
75	95	30	80	48.6	60829	PASS
95	95	100	100	100.0	125208	PASS
96	95	5	9	6.7	8361	PASS
173	174	0.00	2	1.4	1390	PASS
174	95	50	120	81.8	102413	PASS
175	174	5	9	7.4	7561	PASS
176	174	95	101	95.2	97504	PASS
177	176	5	9	6.5	6348	PASS

Scan 2858 (10.080 min): VV006972.D
BFB82

m/z	Abundance
39.90	421.0
43.90	1100.0
76.90	189.0
207.00	152.0

Instrument :
MSVOA_V
ClientSampleId :
BFB82

m/z	Abundance
36.00	1120.0
37.00	5362.0
38.00	4577.0
39.00	2248.0
39.90	592.0
44.00	1576.0
44.90	954.0
46.00	219.0
47.10	1510.0
47.90	925.0
49.00	4859.0
50.00	21648.0
51.00	7778.0
52.00	399.0
53.00	168.0
55.00	432.0
55.90	1442.0
57.00	2845.0
60.00	1106.0
61.00	5546.0
62.00	5618.0
63.00	4807.0
64.00	835.0
65.00	1378.0
66.90	280.0
68.00	11134.0
69.00	12409.0
70.00	989.0
72.00	564.0
73.00	5200.0
74.00	20080.0
75.00	58816.0
76.00	4881.0
76.90	782.0
77.90	540.0
78.90	3268.0
79.90	1158.0
80.90	3378.0
81.90	947.0
82.90	192.0
85.80	239.0
87.00	5696.0
87.90	5682.0
90.80	498.0
92.00	3350.0
93.00	5013.0
94.00	13239.0
95.00	117664.0
96.00	8167.0
97.00	256.0
103.80	451.0
105.90	331.0
106.90	183.0
112.90	144.0
115.80	340.0
116.90	747.0
117.90	384.0
118.80	955.0
125.80	108.0
127.80	248.0
128.80	217.0
129.90	382.0
134.90	210.0
136.70	195.0
139.80	104.0
140.90	1130.0
141.80	178.0
142.90	1620.0
144.90	559.0
145.80	210.0
147.90	266.0
154.80	390.0
156.90	158.0
160.80	133.0
170.80	156.0
171.90	1523.0
173.00	1300.0
173.90	93776.0
174.90	7229.0
175.90	90336.0
176.90	6149.0
178.00	276.0
207.00	131.0

Instrument :
MSVOA_V
ClientSampleId :
BFB82

m/z	Abundance
36.10	1272.0
37.00	5683.0
38.00	4938.0
39.00	2372.0
39.90	585.0
42.00	102.0
44.00	1812.0
44.90	966.0
46.00	226.0
47.00	1576.0
47.90	943.0
49.00	5437.0
50.00	23264.0
51.00	8434.0
52.00	432.0
53.00	159.0
55.00	458.0
55.90	1661.0
57.00	3134.0
60.00	1166.0
61.00	5687.0
62.00	6075.0
63.00	5163.0
63.90	803.0
65.00	1492.0
66.30	111.0
67.00	291.0
68.00	12315.0
69.00	13473.0
70.00	1011.0
72.00	647.0
73.00	5506.0
74.00	21224.0
75.00	62640.0
76.00	5253.0
76.90	764.0
77.90	612.0
78.90	3602.0
79.90	1215.0
80.90	3533.0
81.90	1052.0
82.90	170.0
85.90	188.0
87.00	6124.0
87.90	6295.0
90.80	508.0
92.00	3667.0
93.00	5327.0
94.00	14426.0
95.00	129640.0
96.00	8535.0
97.00	285.0
103.80	496.0
104.00	514.0
105.00	109.0
105.80	363.0
106.90	180.0
112.90	135.0
114.80	103.0
115.90	405.0
116.90	767.0
117.90	375.0
118.80	897.0
127.80	331.0
128.80	245.0
129.80	418.0
130.90	135.0
134.80	236.0
136.80	222.0
139.90	119.0
140.90	1202.0
141.80	184.0
142.90	1729.0
143.70	122.0
144.90	596.0
145.90	260.0
147.80	231.0
151.80	120.0
154.80	398.0
156.90	230.0
160.80	143.0
171.90	1752.0
173.00	1423.0
173.90	105616.0
174.90	7767.0
175.90	100808.0
176.90	6511.0
177.90	229.0
207.00	168.0

Instrument :
MSVOA_V
ClientSampleId :
BFB82

m/z	Abundance
36.10	1336.0
37.00	5708.0
38.00	5027.0
39.00	2357.0
39.90	577.0
42.80	110.0
44.00	2037.0
44.90	1008.0
46.00	238.0
47.00	1600.0
47.90	849.0
49.00	5424.0
50.00	23144.0
51.00	7963.0
51.90	348.0
52.90	127.0
55.00	433.0
56.00	1620.0
57.00	3112.0
60.00	1107.0
61.00	5653.0
62.00	5951.0
63.00	4982.0
63.90	813.0
65.00	1523.0
66.10	104.0
66.90	327.0
68.00	12651.0
69.00	13101.0
70.00	895.0
72.00	620.0
73.00	5401.0
74.00	20720.0
75.00	61032.0
76.00	5275.0
77.00	818.0
77.90	666.0
78.90	3806.0
79.90	1136.0
80.90	3514.0
81.90	1040.0
82.90	116.0
85.90	178.0
87.00	5983.0
87.90	6169.0
90.80	445.0
92.00	3468.0
93.00	5158.0
94.00	14488.0
95.00	128320.0
96.00	8383.0
97.00	295.0
104.00	487.0
104.90	120.0
105.80	405.0
106.90	126.0
112.80	110.0
114.80	114.0
115.90	396.0
116.90	740.0
117.80	334.0
118.90	721.0
123.90	100.0
127.80	408.0
128.80	228.0
129.80	385.0
130.90	172.0
134.80	217.0
136.90	240.0
139.90	114.0
140.90	1126.0
142.00	161.0
142.90	1730.0
143.80	139.0
144.80	566.0
145.90	278.0
147.80	180.0
150.00	103.0
151.80	149.0
154.90	356.0
156.90	271.0
160.90	125.0
171.90	1725.0
173.00	1449.0
173.90	107848.0
174.90	7688.0
175.90	101368.0
176.90	6385.0
177.80	160.0
207.00	199.0

Instrument :
MSVOA_V
ClientSampleId :
BFB82