

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081019\
 Data File : VV012165.D
 Acq On : 09 Aug 2019 22:00
 Operator : SY/MD
 Sample : K4248-02
 Misc : 5mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F2B05

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081019WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.322	65	72	93	rVB2	344272	371766	5.67%	2.141%
2	1.576	145	151	163	rVB	50664	61495	0.94%	0.354%
3	2.052	292	299	309	rBV4	1805	2315	0.04%	0.013%
4	2.129	312	323	335	rBV	141650	203492	3.10%	1.172%
5	2.791	516	529	545	rBV	158136	273206	4.17%	1.574%
6	3.013	596	598	600	rVB	257	61	0.00%	0.000%
7	3.023	600	601	606	rVB2	131	83	0.00%	0.000%
8	3.229	661	665	667	rBV2	287	223	0.00%	0.001%
9	3.270	672	678	680	rBV	134	124	0.00%	0.001%
10	3.283	680	682	686	rBV2	291	189	0.00%	0.001%
11	3.357	702	705	708	rBV2	298	152	0.00%	0.001%
12	3.393	714	716	718	rVB	290	77	0.00%	0.000%
13	3.444	730	732	733	rBV	166	64	0.00%	0.000%
14	3.457	733	736	738	rBV	171	101	0.00%	0.001%
15	3.473	738	741	743	rBV2	141	85	0.00%	0.000%
16	3.640	790	793	795	rBV2	192	127	0.00%	0.001%
17	3.698	808	811	814	rBV	205	160	0.00%	0.001%
18	3.737	820	823	825	rBV	176	99	0.00%	0.001%
19	3.749	825	827	833	rBV2	188	164	0.00%	0.001%
20	3.801	837	843	844	rBV4	830	896	0.01%	0.005%
21	3.958	872	892	928	rBV	2712437	6558855	100.00%	37.779%
22	4.399	1015	1029	1049	rBV	96565	234298	3.57%	1.350%
23	4.598	1089	1091	1094	rVB	376	210	0.00%	0.001%
24	4.621	1094	1098	1099	rBV2	238	150	0.00%	0.001%
25	4.643	1102	1105	1106	rBV	260	155	0.00%	0.001%
26	4.685	1115	1118	1121	rVB	282	126	0.00%	0.001%
27	4.704	1121	1124	1126	rBV2	744	547	0.01%	0.003%
28	4.785	1148	1149	1152	rVB2	172	66	0.00%	0.000%
29	4.807	1152	1156	1158	rBV	198	206	0.00%	0.001%
30	4.872	1174	1176	1177	rBV	154	69	0.00%	0.000%
31	4.936	1193	1196	1199	rVB2	187	120	0.00%	0.001%
32	4.958	1199	1203	1205	rBV	180	136	0.00%	0.001%
33	4.974	1206	1208	1211	rVB2	364	209	0.00%	0.001%
34	4.990	1211	1213	1214	rBV	257	82	0.00%	0.000%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081019\
 Data File : VV012165.D
 Acq On : 09 Aug 2019 22:00
 Operator : SY/MD
 Sample : K4248-02
 Misc : 5mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F2B05

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081019WMA.M
 Title : VOC Analysis

35	5.013	1218	1220	1224	rVB	352	218	0.00%	0.001%
36	5.093	1225	1245	1272	rBV2	238768	604170	9.21%	3.480%
37	5.290	1302	1306	1309	rBV4	943	1025	0.02%	0.006%
38	5.341	1318	1322	1323	rBV	258	148	0.00%	0.001%
39	5.367	1323	1330	1331	rBV3	1095	1137	0.02%	0.007%
40	5.412	1342	1344	1347	rBV	223	123	0.00%	0.001%
41	5.428	1347	1349	1351	rVV	243	102	0.00%	0.001%
42	5.582	1395	1397	1398	rVB	220	63	0.00%	0.000%
43	5.595	1398	1401	1407	rBV2	255	343	0.01%	0.002%
44	5.662	1407	1422	1446	rBV	309486	599955	9.15%	3.456%
45	5.849	1476	1480	1483	rBV2	466	348	0.01%	0.002%
46	5.958	1498	1514	1545	rBV	1589604	3065170	46.73%	17.655%
47	6.116	1552	1563	1577	rBV	124947	240403	3.67%	1.385%
48	6.322	1624	1627	1631	rVB2	301	211	0.00%	0.001%
49	6.338	1631	1632	1633	rBV	248	57	0.00%	0.000%
50	6.354	1633	1637	1640	rVB2	212	144	0.00%	0.001%
51	6.412	1653	1655	1659	rBV2	283	149	0.00%	0.001%
52	6.441	1662	1664	1667	rVV2	242	104	0.00%	0.001%
53	6.508	1682	1685	1686	rBV	160	113	0.00%	0.001%
54	6.640	1724	1726	1730	rVB	291	166	0.00%	0.001%
55	6.662	1730	1733	1734	rVB2	117	59	0.00%	0.000%
56	6.672	1734	1736	1739	rBV	286	227	0.00%	0.001%
57	6.749	1758	1760	1762	rBV	193	72	0.00%	0.000%
58	6.810	1776	1779	1781	rBV2	197	131	0.00%	0.001%
59	6.852	1789	1792	1796	rBV	303	251	0.00%	0.001%
60	6.878	1799	1800	1803	rBV2	135	55	0.00%	0.000%
61	6.936	1816	1818	1820	rVB	247	81	0.00%	0.000%
62	7.029	1834	1847	1864	rBV	72643	127664	1.95%	0.735%
63	7.138	1878	1881	1885	rBV2	380	278	0.00%	0.002%
64	7.241	1910	1913	1918	rBV	164	129	0.00%	0.001%
65	7.299	1928	1931	1933	rBV	169	111	0.00%	0.001%
66	7.357	1936	1949	1967	rBV	291171	494105	7.53%	2.846%
67	7.572	2014	2016	2019	rVB	314	170	0.00%	0.001%
68	7.601	2023	2025	2028	rVB2	223	82	0.00%	0.000%
69	7.662	2034	2044	2064	rBV	50670	84992	1.30%	0.490%
70	7.788	2081	2083	2090	rVB3	517	353	0.01%	0.002%
71	7.926	2123	2126	2128	rBV	262	145	0.00%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081019\
 Data File : VV012165.D
 Acq On : 09 Aug 2019 22:00
 Operator : SY/MD
 Sample : K4248-02
 Misc : 5mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F2B05

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081019WMA.M
 Title : VOC Analysis

72	7.942	2128	2131	2134	rVB	297	169	0.00%	0.001%
73	8.016	2140	2154	2179	rBV	1332134	2213850	33.75%	12.752%
74	8.129	2180	2189	2221	rVB	122822	217564	3.32%	1.253%
75	8.312	2244	2246	2250	rBV2	295	201	0.00%	0.001%
76	8.540	2315	2317	2325	rVB2	281	276	0.00%	0.002%
77	8.621	2338	2342	2344	rBV2	192	174	0.00%	0.001%
78	8.691	2361	2364	2369	rBV2	163	143	0.00%	0.001%
79	8.756	2381	2384	2386	rBV2	158	112	0.00%	0.001%
80	8.791	2392	2395	2397	rBV	223	124	0.00%	0.001%
81	8.894	2414	2427	2450	rBV	427682	701963	10.70%	4.043%
82	9.042	2472	2473	2475	rBV	315	178	0.00%	0.001%
83	9.174	2510	2514	2517	rBV3	424	363	0.01%	0.002%
84	9.412	2587	2588	2590	rBV	234	58	0.00%	0.000%
85	9.457	2599	2602	2606	rBV2	180	193	0.00%	0.001%
86	9.585	2637	2642	2645	rBV	527	498	0.01%	0.003%
87	9.891	2735	2737	2738	rBV	220	104	0.00%	0.001%
88	9.932	2748	2750	2752	rBV	276	139	0.00%	0.001%
89	10.151	2813	2818	2822	rBV2	216	285	0.00%	0.002%
90	10.260	2839	2852	2870	rBV	166017	261266	3.98%	1.505%
91	10.469	2915	2917	2919	rVB	186	69	0.00%	0.000%
92	11.039	3091	3094	3096	rBV	216	150	0.00%	0.001%
93	11.199	3141	3144	3147	rBV	218	122	0.00%	0.001%
94	11.293	3161	3173	3198	rBV	392539	624306	9.52%	3.596%
95	11.669	3278	3290	3311	rBV	253171	404576	6.17%	2.330%
96	11.778	3322	3324	3327	rBV2	198	97	0.00%	0.001%
97	12.289	3481	3483	3484	rBV	274	77	0.00%	0.000%
98	12.456	3531	3535	3540	rBV	364	419	0.01%	0.002%
99	12.479	3541	3542	3543	rVB	251	51	0.00%	0.000%
100	14.257	4092	4095	4097	rBV	479	379	0.01%	0.002%


Sum of corrected areas: 17361068

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV081019\
Data File : VV012165.D
Acq On : 09 Aug 2019 22:00
Operator : SY/MD
Sample : K4248-02
Misc : 5mL/MSVOA V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F2B05

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081019WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

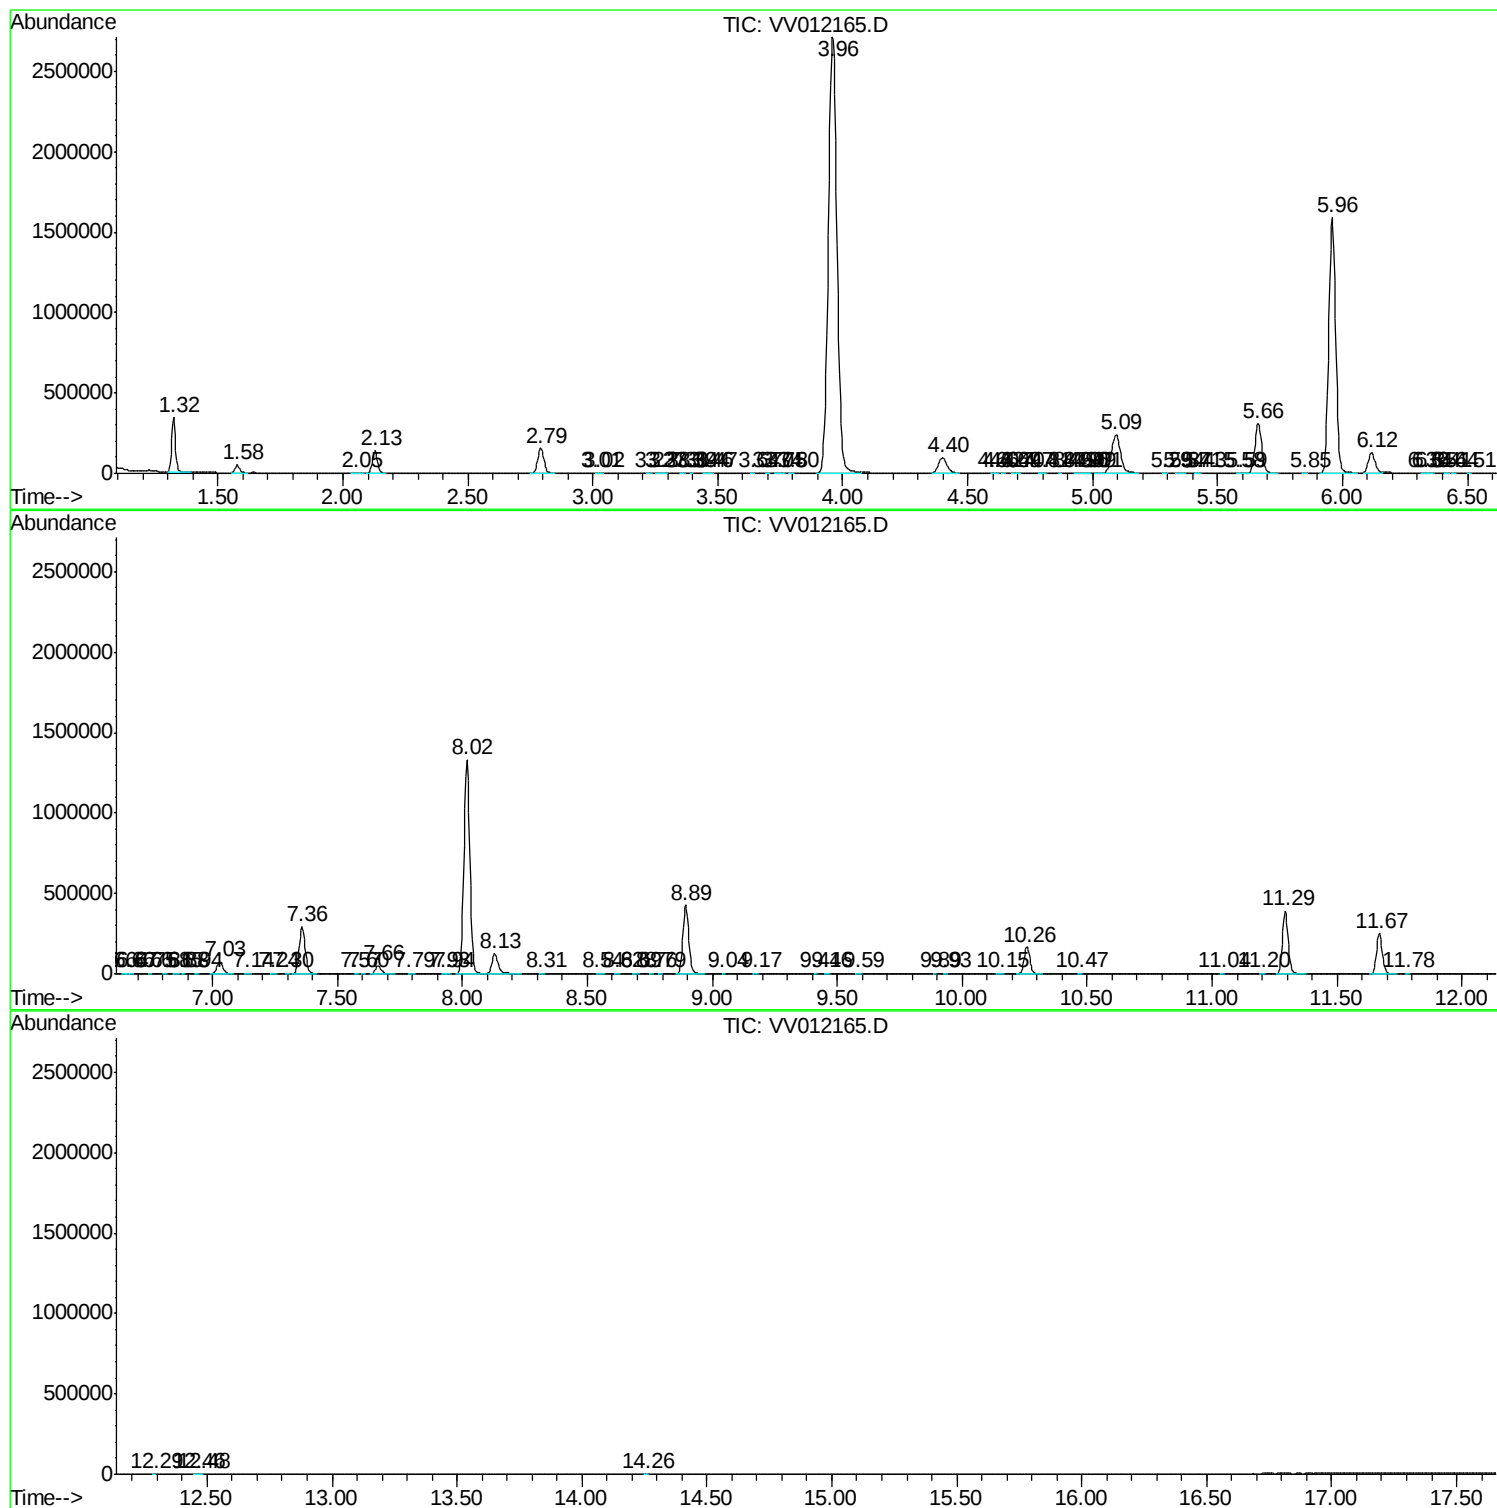

Data_Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV081019\
Data_File : VV012165.D
Acq_On : .09_Aug_2019_ 22:000
Operator : SY/MDD
Sample : K4248-022
Misc : .5mL/MSVOA_V/WATER
ALS_Vial : .14 Sample_Multiplier: .11

Instrument :
MSVOA_V
ClientSampleId :
F2B05

Quant_Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081019WMA.MM
Quant_Title : VOC_Analysis

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	-Internal Standard-	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---------------------	---	----	------	------

No Library Search Compounds Detected
