

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081019\
 Data File : VV012167.D
 Acq On : 09 Aug 2019 22:49
 Operator : SY/MD
 Sample : K4248-04
 Misc : 5mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F2B07

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081019WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.322	65	72	87	rVB2	248735	271843	2.56%	0.988%
2	1.579	145	152	164	rVB	51286	61110	0.58%	0.222%
3	2.129	312	323	335	rBV	140404	199981	1.88%	0.727%
4	2.460	422	426	429	rBV3	424	413	0.00%	0.002%
5	2.528	446	447	450	rBV2	337	153	0.00%	0.001%
6	2.608	461	472	480	rBV5	1812	3168	0.03%	0.012%
7	2.791	517	529	554	rBV	221824	382514	3.60%	1.390%
8	3.097	623	624	625	rVB	145	28	0.00%	0.000%
9	3.225	663	664	665	rVB	195	38	0.00%	0.000%
10	3.241	666	669	673	rBV2	186	188	0.00%	0.001%
11	3.563	767	769	771	rBV	153	110	0.00%	0.000%
12	3.759	827	830	832	rBV	199	131	0.00%	0.000%
13	3.807	833	845	857	rVV2	2324	4641	0.04%	0.017%
14	3.958	872	892	936	rBV	4285015	10378576	97.80%	37.710%
15	4.399	1015	1029	1052	rVB2	97596	239159	2.25%	0.869%
16	4.724	1120	1130	1132	rBV6	2575	3954	0.04%	0.014%
17	4.868	1173	1175	1177	rVB	126	29	0.00%	0.000%
18	4.881	1177	1179	1181	rBV	193	124	0.00%	0.000%
19	4.917	1189	1190	1194	rBV2	237	180	0.00%	0.001%
20	5.097	1228	1246	1273	rBV2	233622	584150	5.50%	2.122%
21	5.293	1304	1307	1310	rVB2	238	187	0.00%	0.001%
22	5.495	1366	1370	1374	rBV2	255	267	0.00%	0.001%
23	5.531	1380	1381	1382	rBV2	217	74	0.00%	0.000%
24	5.572	1392	1394	1395	rBV2	162	69	0.00%	0.000%
25	5.662	1408	1422	1450	rBV	301006	592916	5.59%	2.154%
26	5.958	1497	1514	1551	rBV	5553523	10612552	100.00%	38.560%
27	6.116	1554	1563	1581	rVB2	125847	249411	2.35%	0.906%
28	6.418	1655	1657	1663	rBV2	286	172	0.00%	0.001%
29	6.540	1693	1695	1697	rBV2	297	106	0.00%	0.000%
30	6.669	1734	1735	1736	rVB	226	44	0.00%	0.000%
31	6.682	1736	1739	1741	rBV2	258	213	0.00%	0.001%
32	6.823	1780	1783	1786	rBV2	229	208	0.00%	0.001%
33	6.878	1797	1800	1801	rBV	170	107	0.00%	0.000%
34	7.029	1832	1847	1864	rBV	70617	125200	1.18%	0.455%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081019\
 Data File : VV012167.D
 Acq On : 09 Aug 2019 22:49
 Operator : SY/MD
 Sample : K4248-04
 Misc : 5mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F2B07

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081019WMA.M
 Title : VOC Analysis

35	7.193	1891	1898	1905	rBV	375	576	0.01%	0.002%
36	7.357	1937	1949	1968	rBV	285851	490503	4.62%	1.782%
37	7.553	2008	2010	2013	rVB2	407	214	0.00%	0.001%
38	7.569	2013	2015	2018	rBV2	205	128	0.00%	0.000%
39	7.621	2030	2031	2032	rVB	125	24	0.00%	0.000%
40	7.662	2033	2044	2059	rBV	49381	82898	0.78%	0.301%
41	7.813	2085	2091	2092	rBV	180	170	0.00%	0.001%
42	7.942	2129	2131	2133	rVB	176	71	0.00%	0.000%
43	7.955	2133	2135	2137	rBV2	144	80	0.00%	0.000%
44	8.016	2137	2154	2176	rBV	623705	1037419	9.78%	3.769%
45	8.129	2179	2189	2223	rVB	123518	214686	2.02%	0.780%
46	8.521	2308	2311	2313	rBV	283	209	0.00%	0.001%
47	8.894	2414	2427	2448	rBV	430875	693773	6.54%	2.521%
48	9.084	2484	2486	2488	rVB2	304	152	0.00%	0.001%
49	9.440	2593	2597	2599	rBV	329	259	0.00%	0.001%
50	9.736	2688	2689	2690	rBV	241	63	0.00%	0.000%
51	10.058	2788	2789	2794	rVB2	288	130	0.00%	0.000%
52	10.260	2840	2852	2869	rBV	165768	258202	2.43%	0.938%
53	10.611	2957	2961	2964	rBV2	252	233	0.00%	0.001%
54	10.952	3065	3067	3075	rBV2	380	367	0.00%	0.001%
55	11.074	3103	3105	3107	rVB	278	99	0.00%	0.000%
56	11.228	3149	3153	3158	rBV2	479	535	0.01%	0.002%
57	11.292	3161	3173	3196	rBV	396306	620985	5.85%	2.256%
58	11.669	3277	3290	3308	rBV	255062	407896	3.84%	1.482%
59	12.791	3637	3639	3640	rBV	253	59	0.00%	0.000%
60	14.128	4053	4055	4058	rVB2	607	240	0.00%	0.001%
61	14.148	4058	4061	4063	rBV2	369	242	0.00%	0.001%


Sum of corrected areas: 27522229

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV081019\
Data File : VV012167.D
Acq On : 09 Aug 2019 22:49
Operator : SY/MD
Sample : K4248-04
Misc : 5mL/MSVOA V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
F2B07

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081019WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

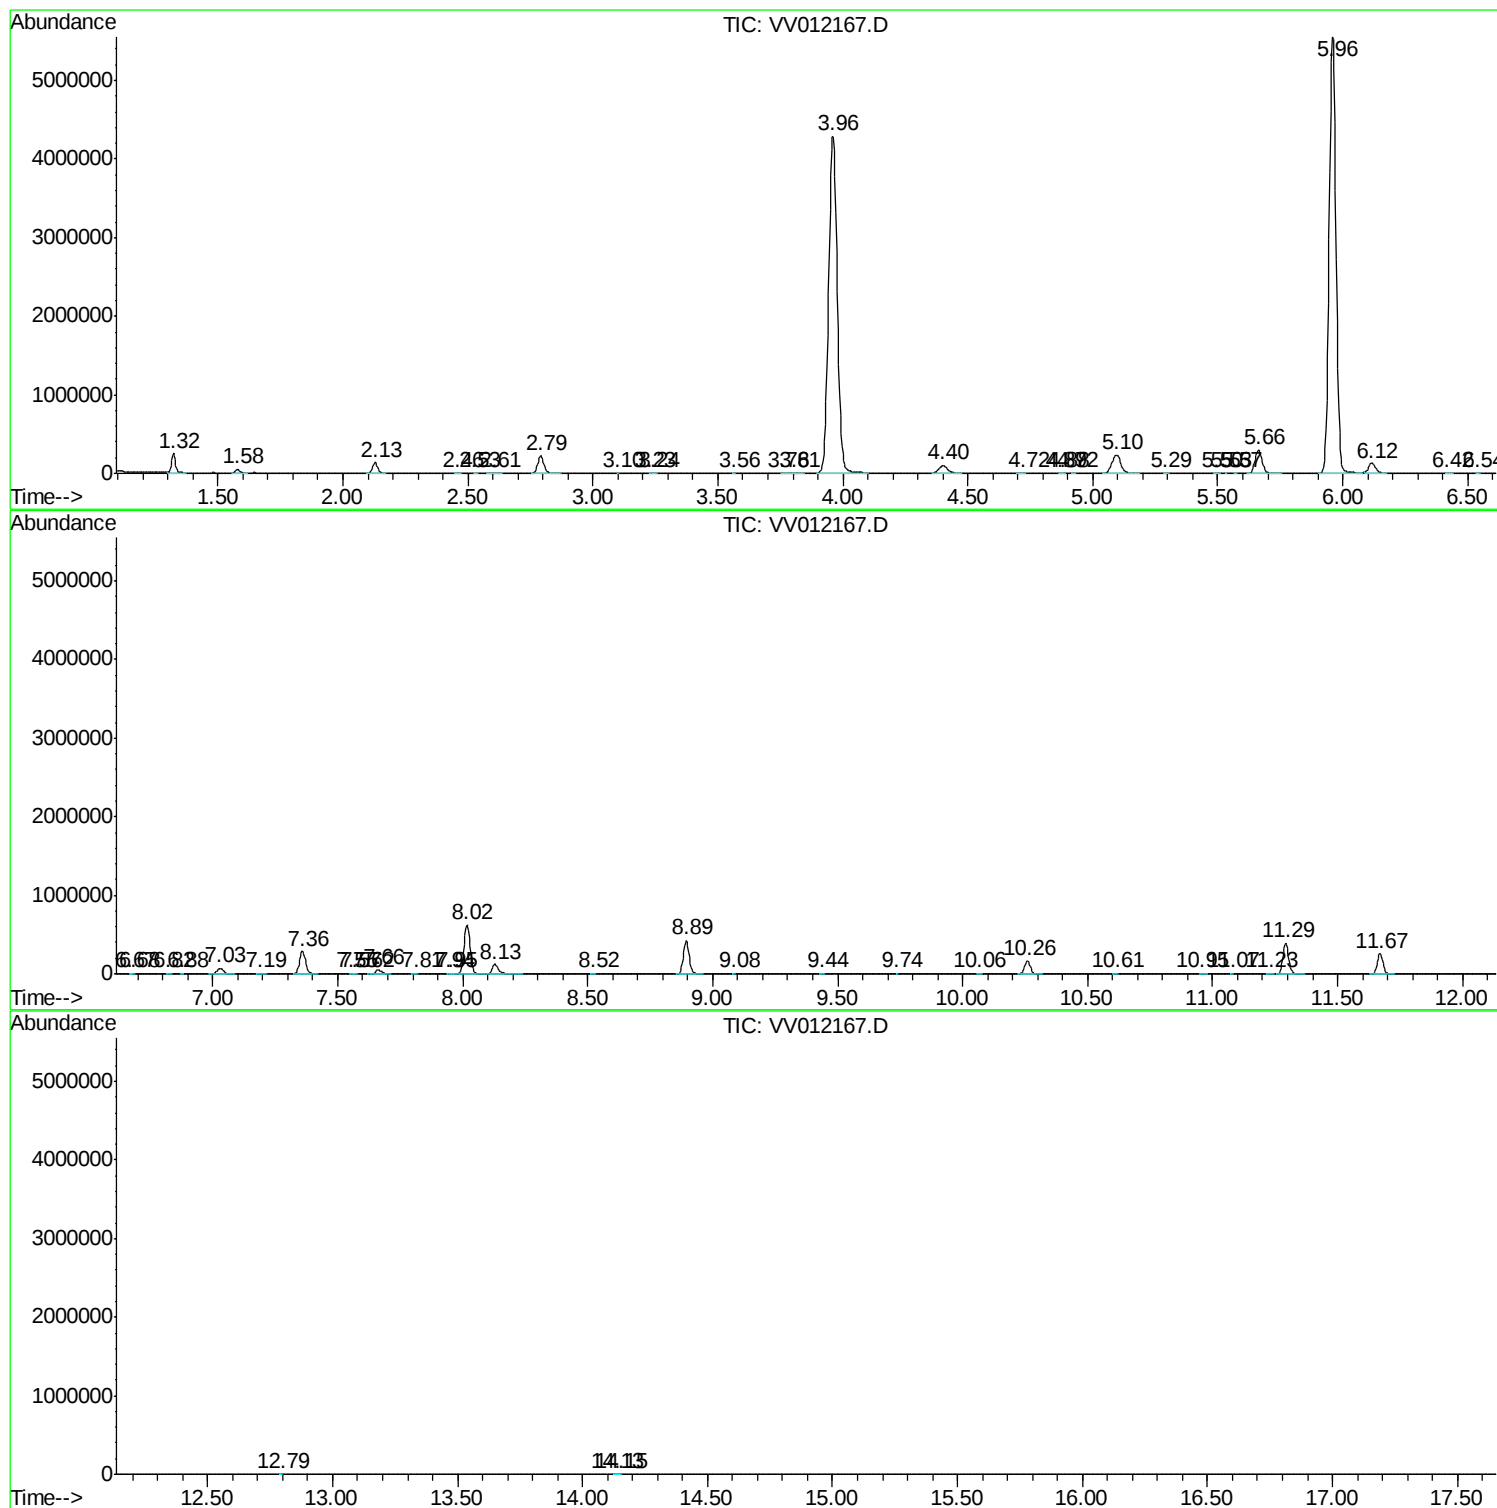

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV081019\
Data File : VV012167.D
Acq On : 09 Aug 2019 22:49
Operator : SY/MD
Sample : K4248-04
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F2B07

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081019WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV081019\
Data File : VV012167.D
Acq On : 09 Aug 2019 22:49
Operator : SY/MD
Sample : K4248-04
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F2B07

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081019WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc