

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081019\
 Data File : VV012177.D
 Acq On : 10 Aug 2019 02:54
 Operator : SY/MD
 Sample : K4248-15
 Misc : 5mL/MSVOA V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F2B53

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081019WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	66	71	79	rVB	73937	71580	10.47%	1.529%
2	1.576	145	151	166	rVB	43696	51751	7.57%	1.106%
3	2.126	313	322	334	rVB	123699	175524	25.69%	3.750%
4	3.087	620	621	622	rBV	145	40	0.01%	0.001%
5	3.251	671	672	673	rVB	186	36	0.01%	0.001%
6	3.264	674	676	677	rVB	251	58	0.01%	0.001%
7	3.299	685	687	689	rBV	184	102	0.01%	0.002%
8	3.531	756	759	762	rBV2	180	183	0.03%	0.004%
9	3.733	820	822	825	rBV2	263	156	0.02%	0.003%
10	3.807	843	845	850	rBV	301	248	0.04%	0.005%
11	3.942	873	887	921	rBV5	22167	82522	12.08%	1.763%
12	4.161	953	955	956	rBV	319	124	0.02%	0.003%
13	4.399	1014	1029	1052	rBV2	84335	215950	31.60%	4.614%
14	4.624	1098	1099	1100	rBV	206	43	0.01%	0.001%
15	4.704	1122	1124	1125	rBV	143	59	0.01%	0.001%
16	4.900	1184	1185	1188	rVB2	149	44	0.01%	0.001%
17	4.984	1200	1211	1214	rBV2	287	441	0.06%	0.009%
18	5.093	1227	1245	1270	rBV3	215911	532610	77.94%	11.380%
19	5.302	1308	1310	1314	rVB2	239	126	0.02%	0.003%
20	5.498	1369	1371	1372	rBV	38	14	0.00%	0.000%
21	5.518	1372	1377	1379	rBV2	433	396	0.06%	0.008%
22	5.662	1407	1422	1448	rBV	293591	577287	84.48%	12.335%
23	6.116	1545	1563	1584	rBV	115395	228948	33.50%	4.892%
24	6.457	1668	1669	1670	rBV	206	64	0.01%	0.001%
25	6.489	1676	1679	1683	rBV2	188	191	0.03%	0.004%
26	6.563	1701	1702	1703	rBB	140	27	0.00%	0.001%
27	6.617	1716	1719	1721	rBV	245	171	0.03%	0.004%
28	6.662	1731	1733	1735	rBV	197	128	0.02%	0.003%
29	6.794	1773	1774	1775	rBB	47	23	0.00%	0.000%
30	6.904	1806	1808	1811	rBV	189	129	0.02%	0.003%
31	6.920	1812	1813	1815	rVB	99	38	0.01%	0.001%
32	6.942	1815	1820	1824	rVB2	272	310	0.05%	0.007%
33	6.961	1824	1826	1827	rBV	54	23	0.00%	0.000%
34	6.977	1829	1831	1832	rBV	154	52	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081019\
 Data File : VV012177.D
 Acq On : 10 Aug 2019 02:54
 Operator : SY/MD
 Sample : K4248-15
 Misc : 5mL/MSVOA V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F2B53

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081019WMA.M
 Title : VOC Analysis

35	7.029	1835	1847	1867	rBV	63356	110417	16.16%	2.359%
36	7.251	1911	1916	1922	rBV2	238	360	0.05%	0.008%
37	7.299	1929	1931	1932	rBV	263	90	0.01%	0.002%
38	7.360	1937	1950	1966	rBV	257830	442922	64.82%	9.464%
39	7.547	2005	2008	2009	rBV	285	173	0.03%	0.004%
40	7.662	2034	2044	2061	rBV2	44592	73990	10.83%	1.581%
41	7.942	2128	2131	2136	rBV	287	316	0.05%	0.007%
42	8.129	2179	2189	2216	rBV	108166	191923	28.09%	4.101%
43	8.357	2258	2260	2263	rVB	257	136	0.02%	0.003%
44	8.402	2271	2274	2275	rBV	199	94	0.01%	0.002%
45	8.701	2362	2367	2370	rBV2	352	378	0.06%	0.008%
46	8.894	2415	2427	2449	rBV	425855	683359	100.00%	14.602%
47	9.083	2484	2486	2488	rBV	308	104	0.02%	0.002%
48	9.212	2521	2526	2527	rBV	285	209	0.03%	0.004%
49	9.260	2537	2541	2544	rBV	257	256	0.04%	0.005%
50	9.878	2731	2733	2735	rBV2	128	76	0.01%	0.002%
51	10.051	2785	2787	2788	rBV	211	62	0.01%	0.001%
52	10.180	2825	2827	2830	rBV	210	123	0.02%	0.003%
53	10.260	2840	2852	2870	rVB	151557	238426	34.89%	5.095%
54	11.006	3082	3084	3086	rBV	233	80	0.01%	0.002%
55	11.093	3109	3111	3114	rBV	336	117	0.02%	0.002%
56	11.157	3129	3131	3136	rVB2	271	104	0.02%	0.002%
57	11.292	3161	3173	3194	rBV	389158	612582	89.64%	13.089%
58	11.431	3215	3216	3221	rVB2	461	274	0.04%	0.006%
59	11.669	3278	3290	3307	rBV	241698	383733	56.15%	8.199%
60	15.334	4428	4430	4434	rBV2	575	357	0.05%	0.008%


Sum of corrected areas: 4680059

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV081019\
Data File : VV012177.D
Acq On : 10 Aug 2019 02:54
Operator : SY/MD
Sample : K4248-15
Misc : 5mL/MSVOA V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F2B53

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081019WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

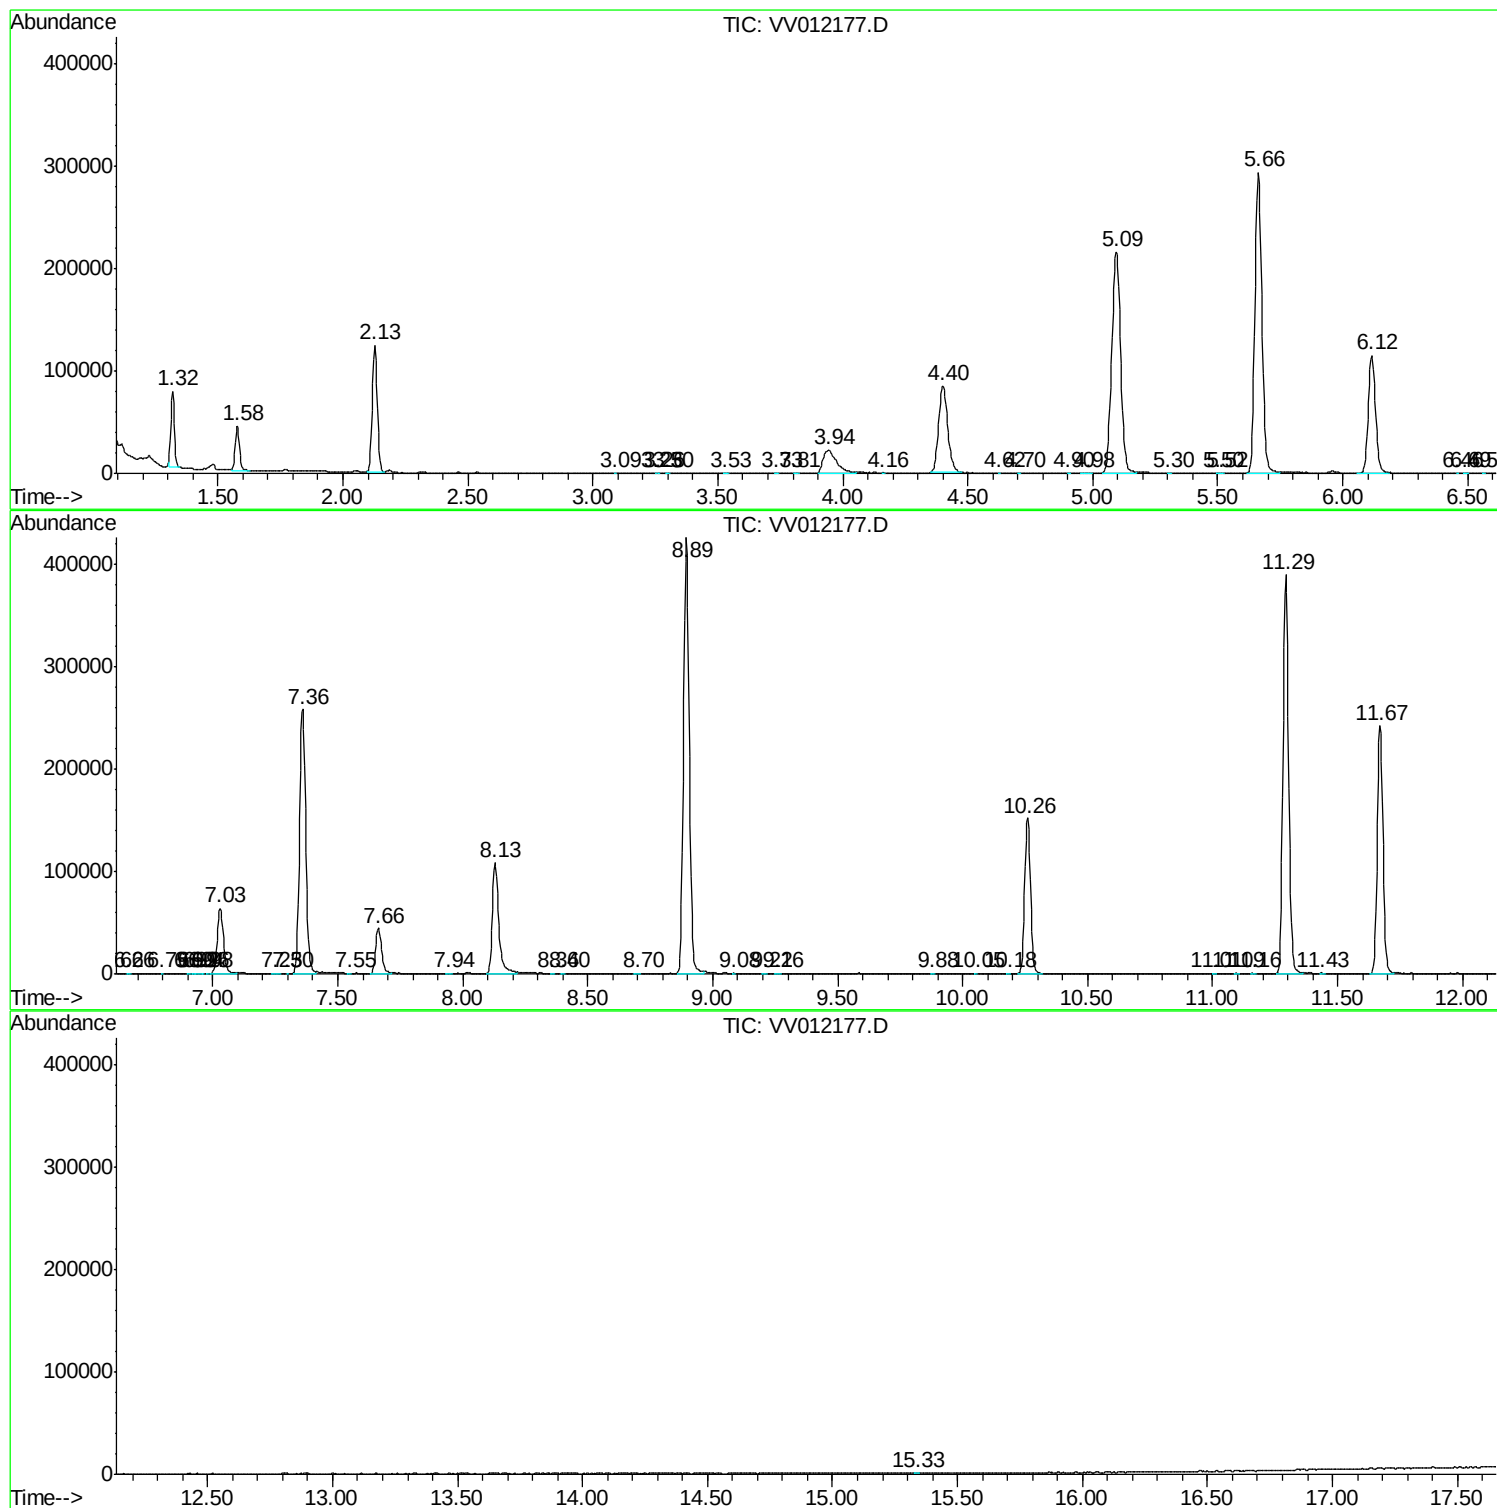

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV081019\
Data File : VV012177.D
Acq On : 10 Aug 2019 02:54
Operator : SY/MD
Sample : K4248-15
Misc : 5mL/MSV0A_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
F2B53

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM081019WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV081019\
Data File : VV012177.D
Acq On : 10 Aug 2019 02:54
Operator : SY/MD
Sample : K4248-15
Misc : 5mL/MSV0A_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
F2B53

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM081019WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
