

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081019\
 Data File : VV012181.D
 Acq On : 10 Aug 2019 04:32
 Operator : SY/MD
 Sample : K4248-19
 Misc : 5mL/MSVOA V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F2B60

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081019WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	65	71	86	rVB	71688	74728	10.94%	1.617%
2	1.576	144	151	168	rVB	43974	54890	8.03%	1.188%
3	2.126	313	322	335	rBV	122122	172253	25.21%	3.728%
4	2.457	422	425	428	rBV2	430	291	0.04%	0.006%
5	2.534	443	449	453	rBV3	413	450	0.07%	0.010%
6	2.749	514	516	518	rBV	159	51	0.01%	0.001%
7	2.865	545	552	555	rBV2	236	347	0.05%	0.008%
8	2.878	555	556	558	rVB	240	95	0.01%	0.002%
9	2.955	578	580	581	rBV	319	120	0.02%	0.003%
10	3.029	600	603	606	rBV2	244	213	0.03%	0.005%
11	3.180	647	650	654	rBV2	185	155	0.02%	0.003%
12	3.373	708	710	711	rVB	152	34	0.00%	0.001%
13	3.441	729	731	734	rBV	137	93	0.01%	0.002%
14	3.460	734	737	740	rBV2	218	179	0.03%	0.004%
15	3.569	768	771	773	rBV2	197	166	0.02%	0.004%
16	3.608	780	783	785	rBV2	178	135	0.02%	0.003%
17	3.740	823	824	827	rBV2	103	67	0.01%	0.001%
18	3.827	850	851	852	rBV2	80	26	0.00%	0.001%
19	3.955	872	891	923	rBV7	18657	81475	11.93%	1.763%
20	4.119	940	942	947	rVB2	244	126	0.02%	0.003%
21	4.302	997	999	1001	rVB	197	54	0.01%	0.001%
22	4.399	1012	1029	1054	rBV	84552	215598	31.56%	4.667%
23	4.688	1118	1119	1120	rBV	81	29	0.00%	0.001%
24	4.788	1147	1150	1152	rBV2	175	130	0.02%	0.003%
25	4.846	1166	1168	1170	rBV	133	85	0.01%	0.002%
26	4.904	1183	1186	1189	rBV	231	177	0.03%	0.004%
27	4.929	1192	1194	1198	rBV	169	135	0.02%	0.003%
28	4.958	1198	1203	1206	rBV	237	203	0.03%	0.004%
29	4.974	1206	1208	1209	rBV	134	63	0.01%	0.001%
30	4.997	1209	1215	1216	rBV2	182	171	0.03%	0.004%
31	5.093	1227	1245	1273	rBV3	209755	523901	76.69%	11.340%
32	5.267	1297	1299	1300	rBV	196	46	0.01%	0.001%
33	5.331	1318	1319	1320	rVB	411	79	0.01%	0.002%
34	5.344	1320	1323	1324	rBV	191	91	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081019\
 Data File : VV012181.D
 Acq On : 10 Aug 2019 04:32
 Operator : SY/MD
 Sample : K4248-19
 Misc : 5mL/MSVOA V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F2B60

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081019WMA.M
 Title : VOC Analysis

35	5.354	1324	1326	1329	rBV	195	124	0.02%	0.003%
36	5.518	1374	1377	1378	rBV	202	102	0.01%	0.002%
37	5.662	1406	1422	1447	rBV	295870	577468	84.53%	12.499%
38	5.843	1476	1478	1483	rVB2	353	151	0.02%	0.003%
39	5.990	1523	1524	1528	rBV2	183	121	0.02%	0.003%
40	6.039	1536	1539	1540	rBV	134	73	0.01%	0.002%
41	6.071	1548	1549	1550	rBV	217	50	0.01%	0.001%
42	6.116	1550	1563	1585	rVV	110148	221687	32.45%	4.798%
43	6.209	1590	1592	1593	rBV	210	50	0.01%	0.001%
44	6.235	1599	1600	1603	rBV	222	127	0.02%	0.003%
45	6.453	1664	1668	1670	rBV2	299	247	0.04%	0.005%
46	6.621	1712	1720	1725	rBV4	835	1065	0.16%	0.023%
47	6.691	1740	1742	1744	rBV	206	136	0.02%	0.003%
48	6.778	1766	1769	1771	rBB	57	30	0.00%	0.001%
49	6.804	1771	1777	1780	rBV2	242	266	0.04%	0.006%
50	6.817	1780	1781	1782	rBV2	113	43	0.01%	0.001%
51	6.942	1816	1820	1822	rBV2	290	223	0.03%	0.005%
52	7.029	1836	1847	1864	rBV2	61309	105231	15.40%	2.278%
53	7.145	1881	1883	1887	rBV	276	255	0.04%	0.006%
54	7.228	1907	1909	1910	rBV	133	40	0.01%	0.001%
55	7.357	1936	1949	1969	rBV	253403	436590	63.91%	9.450%
56	7.566	2012	2014	2018	rVB3	352	241	0.04%	0.005%
57	7.601	2022	2025	2028	rBV	285	197	0.03%	0.004%
58	7.621	2029	2031	2032	rBV	117	45	0.01%	0.001%
59	7.662	2032	2044	2064	rBV2	43207	72876	10.67%	1.577%
60	7.788	2080	2083	2086	rBV2	323	137	0.02%	0.003%
61	7.923	2122	2125	2130	rBV2	269	226	0.03%	0.005%
62	8.019	2152	2155	2160	rVB2	450	413	0.06%	0.009%
63	8.087	2172	2176	2178	rBV2	284	255	0.04%	0.006%
64	8.129	2178	2189	2219	rVV2	101902	191139	27.98%	4.137%
65	8.418	2277	2279	2283	rBV	348	198	0.03%	0.004%
66	8.489	2300	2301	2303	rBV	213	47	0.01%	0.001%
67	8.637	2344	2347	2351	rBV2	271	150	0.02%	0.003%
68	8.894	2415	2427	2453	rBV	420879	683161	100.00%	14.787%
69	9.103	2488	2492	2497	rBV3	545	591	0.09%	0.013%
70	9.158	2507	2509	2510	rBV	121	61	0.01%	0.001%
71	9.190	2514	2519	2523	rVB4	390	425	0.06%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081019\
 Data File : VV012181.D
 Acq On : 10 Aug 2019 04:32
 Operator : SY/MD
 Sample : K4248-19
 Misc : 5mL/MSVOA V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F2B60

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081019WMA.M
 Title : VOC Analysis

72	9.312	2554	2557	2560	rBV	239	160	0.02%	0.003%
73	9.395	2579	2583	2584	rBV2	206	138	0.02%	0.003%
74	10.138	2812	2814	2815	rBV	209	88	0.01%	0.002%
75	10.260	2840	2852	2872	rVB	144881	229331	33.57%	4.964%
76	10.408	2896	2898	2900	rBV	260	150	0.02%	0.003%
77	10.646	2970	2972	2973	rVB2	225	49	0.01%	0.001%
78	11.106	3112	3115	3120	rVB	296	249	0.04%	0.005%
79	11.292	3161	3173	3194	rBV	378279	601418	88.03%	13.017%
80	11.408	3208	3209	3216	rBV2	294	214	0.03%	0.005%
81	11.669	3279	3290	3306	rBV	228760	366075	53.59%	7.924%
82	11.813	3333	3335	3338	rBV	253	87	0.01%	0.002%
83	12.009	3393	3396	3398	rBV	208	143	0.02%	0.003%
84	12.707	3612	3613	3616	rVB	316	143	0.02%	0.003%
85	13.141	3745	3748	3753	rBV2	222	239	0.03%	0.005%
86	13.164	3753	3755	3760	rVB	291	177	0.03%	0.004%
87	13.559	3877	3878	3879	rBV	245	55	0.01%	0.001%
88	13.569	3879	3881	3884	rBV2	278	192	0.03%	0.004%
89	13.733	3929	3932	3935	rBV	401	273	0.04%	0.006%


Sum of corrected areas: 4620078

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV081019\
Data File : VV012181.D
Acq On : 10 Aug 2019 04:32
Operator : SY/MD
Sample : K4248-19
Misc : 5mL/MSVOA V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F2B60

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081019WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

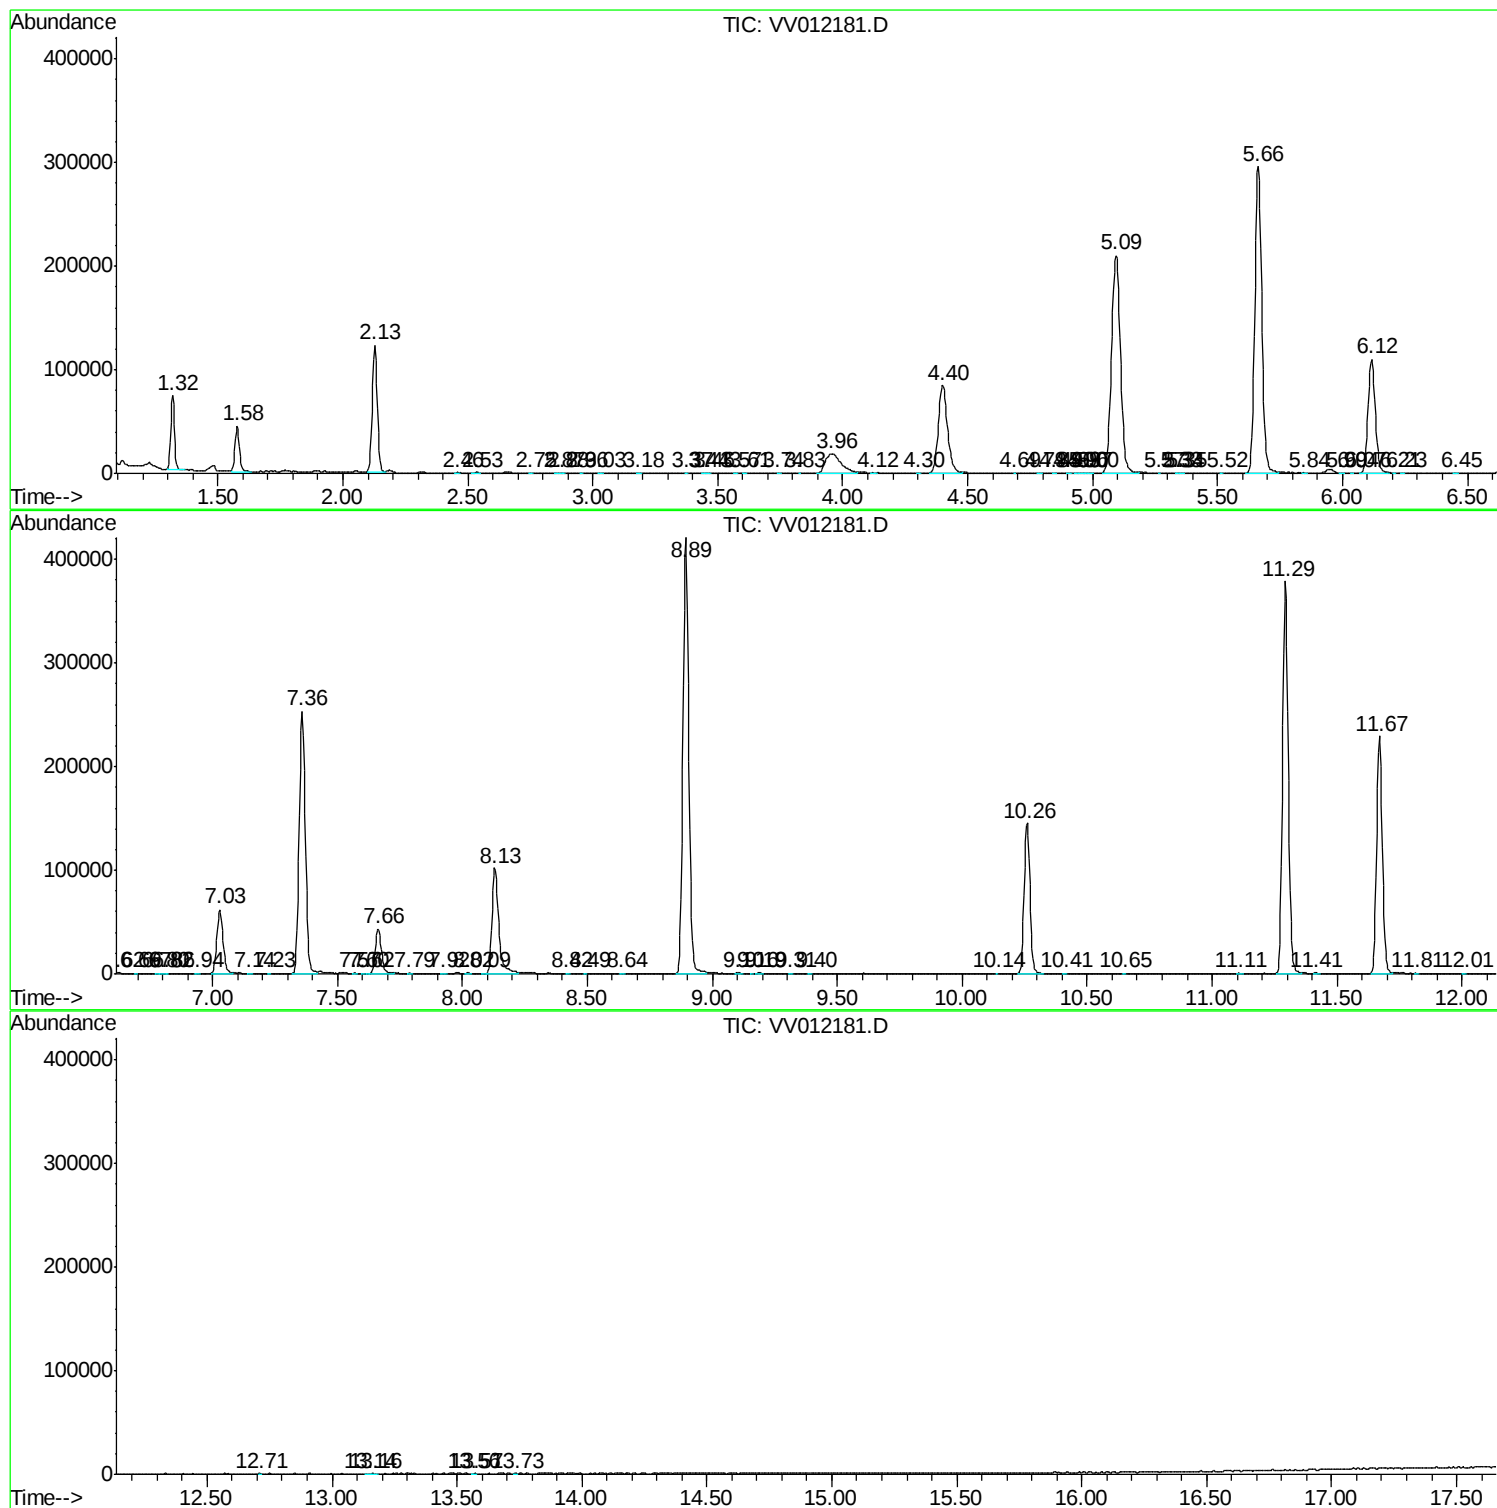

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV081019\
Data File : VV012181.D
Acq On : 10 Aug 2019 04:32
Operator : SY/MD
Sample : K4248-19
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F2B60

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081019WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV081019\
Data File : VV012181.D
Acq On : 10 Aug 2019 04:32
Operator : SY/MD
Sample : K4248-19
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F2B60

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081019WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc