


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV081019\
 Data File : VV012155.D
 Acq On : 09 Aug 2019 16:01
 Operator : SY/MD
 Sample : BFB63
 Misc : 5mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB63

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081019WMA.M
 Title : VOC Analysis
 Last Update : Mon Aug 12 19:05:41 2019

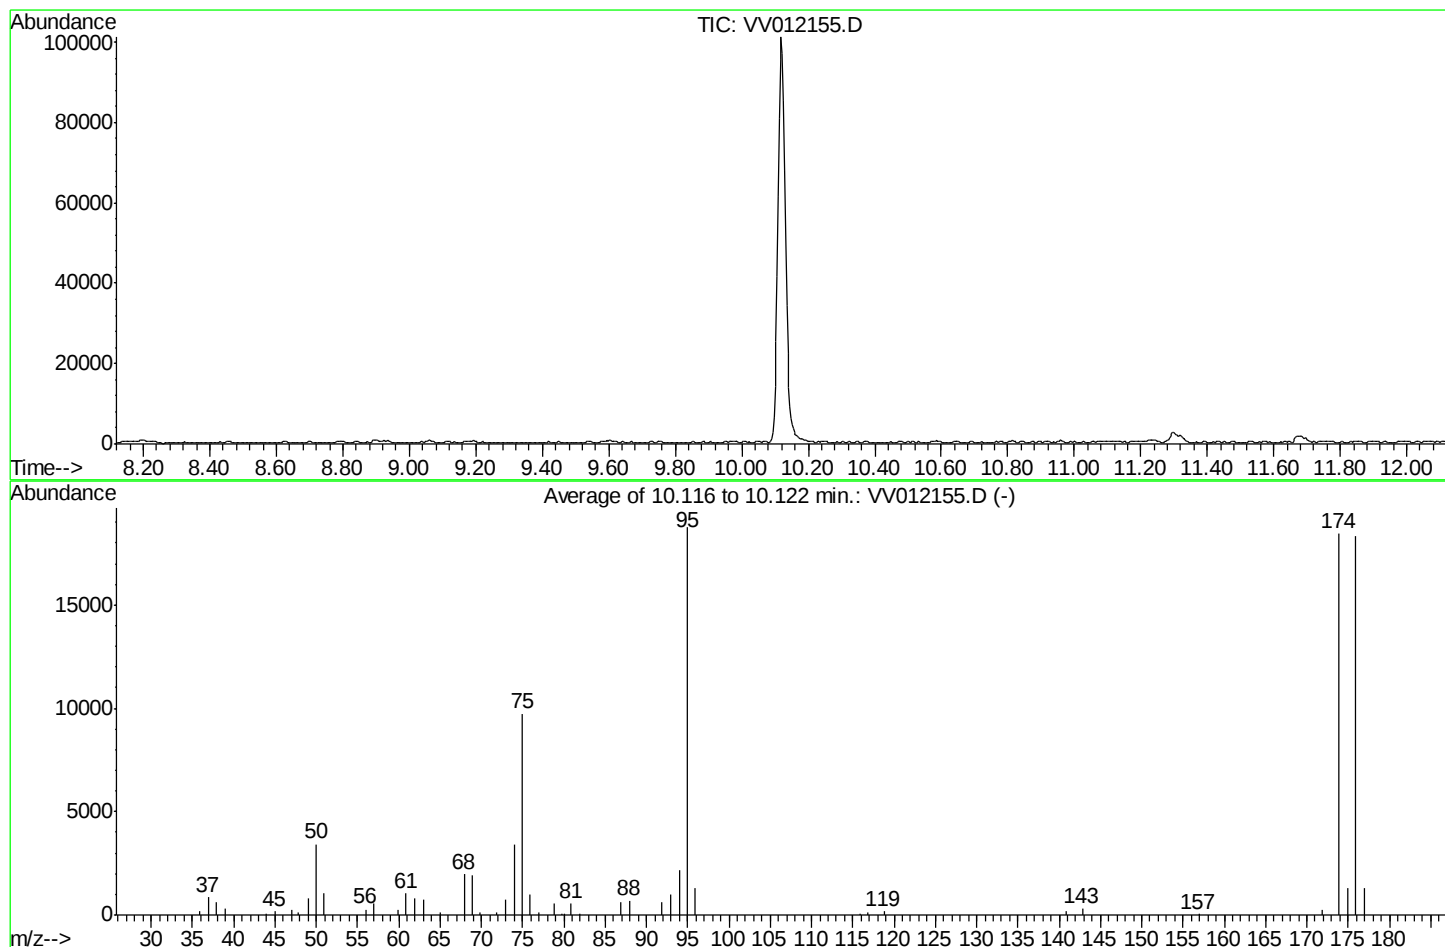

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	3423	PASS
75	95	30	80	51.9	9726	PASS
95	95	100	100	100.0	18757	PASS
96	95	5	9	7.0	1314	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	98.3	18432	PASS
175	174	5	9	7.2	1324	PASS
176	174	95	101	99.4	18314	PASS
177	176	5	9	7.0	1282	PASS

m/z	Abundance
35.80	177.0
36.90	867.0
38.00	626.0
38.90	274.0
39.80	277.0
43.90	224.0
45.00	188.0
47.10	250.0
47.90	165.0
49.00	744.0
50.00	3418.0
50.90	1032.0
56.00	235.0
56.90	503.0
59.90	216.0
60.90	1001.0
62.00	792.0
63.00	787.0
65.00	108.0
68.00	1842.0
68.90	1821.0
70.00	144.0
71.80	116.0
72.90	740.0
74.00	3426.0
75.00	9552.0
75.90	974.0
77.00	171.0
78.80	574.0
79.80	108.0
80.90	624.0
81.80	127.0
86.90	625.0
87.90	705.0
91.90	625.0
92.90	1037.0
94.00	2273.0
95.00	18520.0
95.90	1300.0
116.70	167.0
118.80	196.0
140.90	167.0
142.90	247.0
171.90	218.0
173.90	17896.0
174.90	1303.0
175.90	16920.0
176.90	1249.0

Instrument :
MSVOA_V
ClientSampleId :
BFB63

m/z	Abundance
35.80	217.0
37.00	888.0
37.90	647.0
38.90	288.0
39.80	226.0
43.90	254.0
45.00	171.0
47.10	267.0
47.90	150.0
49.00	806.0
50.00	3536.0
50.90	1119.0
56.00	263.0
56.90	541.0
59.90	228.0
60.90	1084.0
62.00	832.0
63.00	750.0
65.00	136.0
68.00	2058.0
69.00	1918.0
69.80	137.0
71.80	118.0
72.90	756.0
73.90	3454.0
75.00	10000.0
75.90	1039.0
77.00	145.0
78.80	561.0
79.80	106.0
80.90	571.0
81.90	109.0
86.90	642.0
87.90	734.0
91.90	586.0
92.90	996.0
94.00	2267.0
95.00	19360.0
95.90	1360.0
115.90	115.0
116.70	152.0
118.80	176.0
140.90	211.0
142.90	292.0
171.90	266.0
173.90	19104.0
174.90	1384.0
175.90	18968.0
176.90	1307.0

Instrument :
MSVOA_V
ClientSampleId :
BFB63

m/z	Abundance
35.80	210.0
37.00	816.0
37.90	657.0
39.00	299.0
39.80	193.0
43.90	300.0
45.00	135.0
47.10	209.0
47.80	139.0
49.00	783.0
50.00	3315.0
50.90	1056.0
56.00	246.0
56.90	594.0
59.90	214.0
60.90	1048.0
62.00	770.0
62.90	658.0
65.00	152.0
67.90	1967.0
69.00	1950.0
69.80	110.0
71.80	120.0
72.90	758.0
73.90	3263.0
75.00	9626.0
75.90	911.0
78.80	514.0
80.00	112.0
80.80	476.0
86.90	657.0
87.90	633.0
91.90	578.0
93.00	858.0
94.00	2006.0
95.00	18392.0
95.90	1284.0
115.90	128.0
116.80	136.0
118.80	121.0
140.80	237.0
142.80	318.0
156.90	112.0
171.90	310.0
173.90	18296.0
174.90	1285.0
175.90	19056.0
176.90	1290.0

Instrument :
MSVOA_V
ClientSampleId :
BFB63

Scan 2796 (10.080 min): VV012155.D
BFB63

m/z	Abundance
40.00	247.0
44.00	192.0

Instrument :
MSVOA_V
ClientSampleId :
BFB63