


Data Path : Z:\VOASRV\HPCHEM1\MSVOA\_V\DATA\VV081020\  
 Data File : VV017883.D  
 Acq On : 10 Aug 2020 08:55  
 Operator : SY/MD  
 Sample : BFB70  
 Misc : 5.0mL/MSVOA\_V/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 BFB70

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_V\METHOD\SOMVLM080820WMA.M  
 Title : VOC Analysis  
 Last Update : Tue Aug 11 01:17:50 2020

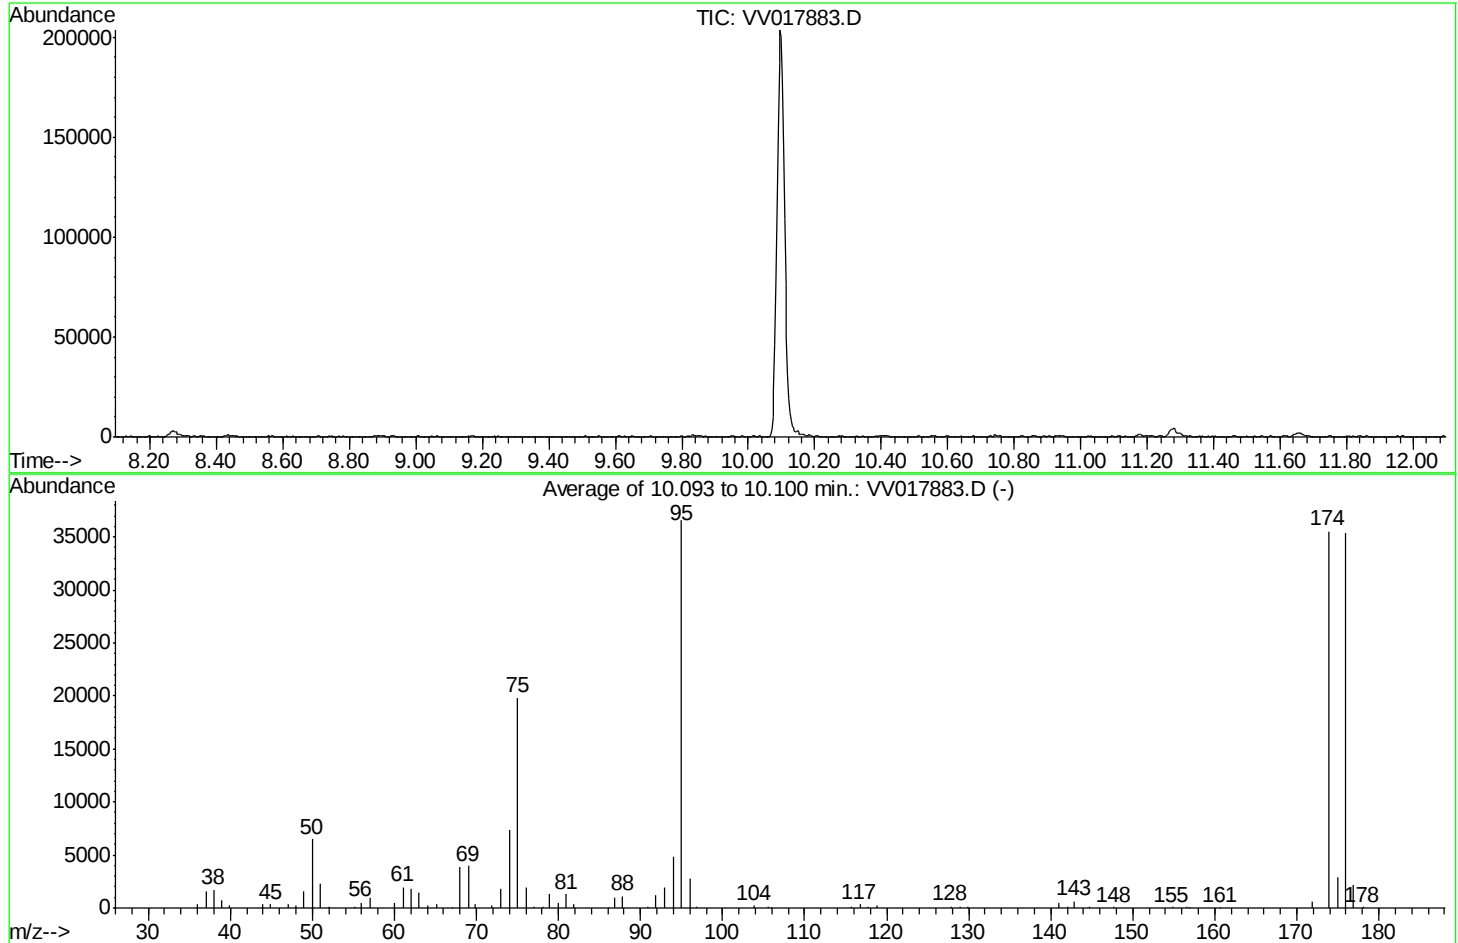

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2789

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 17.7      | 6480    | PASS             |
| 75          | 95           | 30           | 80           | 54.2      | 19818   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 36560   | PASS             |
| 96          | 95           | 5            | 9            | 7.5       | 2724    | PASS             |
| 173         | 174          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 174         | 95           | 50           | 120          | 97.2      | 35528   | PASS             |
| 175         | 174          | 5            | 9            | 8.2       | 2897    | PASS             |
| 176         | 174          | 95           | 101          | 99.6      | 35397   | PASS             |
| 177         | 176          | 5            | 9            | 6.0       | 2133    | PASS             |

| m/z   | Abundance |
|-------|-----------|
| 36.40 | 105.0     |

Instrument :  
MSVOA\_V  
ClientSampleId :  
BFB70

| m/z    | Abundance |
|--------|-----------|
| 36.00  | 301.0     |
| 37.00  | 1473.0    |
| 38.00  | 1612.0    |
| 39.00  | 676.0     |
| 39.90  | 163.0     |
| 43.90  | 251.0     |
| 44.90  | 297.0     |
| 47.10  | 233.0     |
| 48.00  | 219.0     |
| 49.00  | 1566.0    |
| 50.00  | 6317.0    |
| 51.00  | 2210.0    |
| 55.90  | 581.0     |
| 57.00  | 938.0     |
| 59.90  | 442.0     |
| 61.00  | 1776.0    |
| 62.00  | 1630.0    |
| 63.00  | 1432.0    |
| 64.00  | 265.0     |
| 65.10  | 333.0     |
| 68.00  | 3712.0    |
| 69.00  | 3724.0    |
| 69.90  | 355.0     |
| 71.90  | 211.0     |
| 73.00  | 1706.0    |
| 74.00  | 6907.0    |
| 75.00  | 19384.0   |
| 76.00  | 1917.0    |
| 78.10  | 142.0     |
| 78.90  | 1187.0    |
| 79.90  | 452.0     |
| 81.00  | 1348.0    |
| 81.80  | 345.0     |
| 86.80  | 1041.0    |
| 87.80  | 1064.0    |
| 91.00  | 204.0     |
| 91.90  | 1209.0    |
| 92.90  | 1885.0    |
| 94.00  | 4539.0    |
| 95.00  | 34904.0   |
| 96.00  | 2556.0    |
| 96.80  | 147.0     |
| 103.90 | 225.0     |
| 105.60 | 158.0     |
| 115.90 | 127.0     |
| 116.80 | 299.0     |
| 117.80 | 138.0     |
| 118.90 | 154.0     |
| 127.80 | 164.0     |
| 130.10 | 126.0     |
| 141.00 | 422.0     |
| 142.00 | 135.0     |
| 142.90 | 707.0     |
| 144.70 | 192.0     |
| 154.80 | 192.0     |
| 156.90 | 107.0     |
| 171.90 | 565.0     |
| 173.90 | 33680.0   |
| 175.00 | 2565.0    |
| 175.90 | 33488.0   |
| 176.90 | 2034.0    |
| 178.10 | 112.0     |

Instrument :  
MSVOA\_V  
ClientSampleId :  
BFB70

| m/z    | Abundance |
|--------|-----------|
| 36.00  | 390.0     |
| 37.00  | 1536.0    |
| 38.00  | 1768.0    |
| 39.00  | 712.0     |
| 39.90  | 215.0     |
| 43.90  | 335.0     |
| 44.90  | 359.0     |
| 47.10  | 406.0     |
| 47.90  | 280.0     |
| 49.00  | 1636.0    |
| 50.00  | 6553.0    |
| 50.90  | 2406.0    |
| 52.10  | 140.0     |
| 55.20  | 133.0     |
| 55.90  | 493.0     |
| 57.00  | 997.0     |
| 60.00  | 489.0     |
| 61.10  | 2080.0    |
| 62.00  | 1884.0    |
| 63.00  | 1523.0    |
| 64.00  | 285.0     |
| 65.10  | 438.0     |
| 67.00  | 107.0     |
| 68.00  | 4001.0    |
| 69.00  | 4053.0    |
| 69.90  | 369.0     |
| 71.90  | 178.0     |
| 73.00  | 1905.0    |
| 74.00  | 7606.0    |
| 75.00  | 20672.0   |
| 76.00  | 1937.0    |
| 77.00  | 149.0     |
| 78.00  | 191.0     |
| 78.90  | 1409.0    |
| 79.90  | 516.0     |
| 80.90  | 1323.0    |
| 81.80  | 414.0     |
| 86.80  | 1011.0    |
| 87.90  | 1128.0    |
| 91.00  | 152.0     |
| 91.90  | 1291.0    |
| 92.90  | 1977.0    |
| 94.00  | 4968.0    |
| 95.00  | 37744.0   |
| 96.00  | 2799.0    |
| 96.80  | 137.0     |
| 103.90 | 187.0     |
| 105.60 | 167.0     |
| 115.70 | 145.0     |
| 116.80 | 363.0     |
| 117.80 | 168.0     |
| 118.90 | 205.0     |
| 127.80 | 166.0     |
| 128.90 | 144.0     |
| 129.90 | 125.0     |
| 140.90 | 458.0     |
| 142.00 | 145.0     |
| 142.90 | 641.0     |
| 144.80 | 184.0     |
| 147.80 | 110.0     |
| 154.80 | 138.0     |
| 156.60 | 114.0     |
| 160.70 | 108.0     |
| 171.90 | 700.0     |
| 173.90 | 36616.0   |
| 175.00 | 2915.0    |
| 175.90 | 36512.0   |
| 176.90 | 2137.0    |
| 178.10 | 110.0     |

Instrument :  
MSVOA\_V  
ClientSampleId :  
BFB70

| m/z    | Abundance |
|--------|-----------|
| 36.00  | 352.0     |
| 37.00  | 1573.0    |
| 38.00  | 1750.0    |
| 39.00  | 664.0     |
| 39.90  | 239.0     |
| 43.90  | 376.0     |
| 44.90  | 357.0     |
| 47.10  | 421.0     |
| 47.90  | 310.0     |
| 49.00  | 1622.0    |
| 50.00  | 6572.0    |
| 50.90  | 2217.0    |
| 52.00  | 164.0     |
| 55.20  | 137.0     |
| 55.90  | 410.0     |
| 57.00  | 1021.0    |
| 60.00  | 520.0     |
| 61.00  | 2048.0    |
| 62.00  | 1965.0    |
| 62.90  | 1530.0    |
| 64.00  | 273.0     |
| 65.10  | 496.0     |
| 68.00  | 3777.0    |
| 69.00  | 4059.0    |
| 69.90  | 349.0     |
| 71.90  | 207.0     |
| 73.00  | 1969.0    |
| 74.00  | 7433.0    |
| 75.00  | 19400.0   |
| 76.00  | 1804.0    |
| 77.00  | 246.0     |
| 78.00  | 160.0     |
| 78.90  | 1498.0    |
| 79.90  | 471.0     |
| 80.90  | 1256.0    |
| 81.80  | 400.0     |
| 86.00  | 162.0     |
| 86.90  | 942.0     |
| 87.90  | 1151.0    |
| 90.90  | 121.0     |
| 91.90  | 1290.0    |
| 92.90  | 1808.0    |
| 94.00  | 4897.0    |
| 95.00  | 37032.0   |
| 96.00  | 2818.0    |
| 96.80  | 104.0     |
| 103.90 | 181.0     |
| 105.80 | 159.0     |
| 115.70 | 185.0     |
| 116.80 | 369.0     |
| 117.70 | 213.0     |
| 118.80 | 251.0     |
| 127.80 | 171.0     |
| 128.90 | 113.0     |
| 129.90 | 129.0     |
| 140.90 | 484.0     |
| 142.00 | 111.0     |
| 142.90 | 572.0     |
| 144.80 | 171.0     |
| 147.70 | 132.0     |
| 156.50 | 107.0     |
| 171.90 | 715.0     |
| 173.90 | 36288.0   |
| 174.90 | 3213.0    |
| 175.90 | 36192.0   |
| 176.90 | 2230.0    |

Instrument :  
MSVOA\_V  
ClientSampleId :  
BFB70