

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081022\
 Data File : VV027253.D
 Acq On : 10 Aug 2022 12:11
 Operator : SY/MD
 Sample : VV0810WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK257

Quant Time: Aug 11 03:53:31 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Aug 09 02:29:12 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	439768	50.000	ug/L	# 0.00
28) Chlorobenzene-d5	8.850	117	438685	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	195690	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	141975	47.353	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	94.700%
7) Chloroethane-d5	1.558	69	108035	49.289	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	98.580%
11) 1,1-Dichloroethene-d2	2.101	63	192997	35.191	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	70.380%
21) 2-Butanone-d5	3.870	46	222992	83.555	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	83.550%
24) Chloroform-d	4.342	84	255578	41.614	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	83.220%
26) 1,2-Dichloroethane-d4	5.027	65	170869	44.811	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.620%
32) Benzene-d6	5.043	84	550348	52.315	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	104.620%
36) 1,2-Dichloropropane-d6	6.066	67	184607	49.332	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	98.660%
41) Toluene-d8	7.313	98	485081	54.097	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	108.200%
43) trans-1,3-Dichloroprop...	7.619	79	78659	48.224	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	96.440%
47) 2-Hexanone-d5	8.085	63	150186	83.328	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	83.330%
56) 1,1,2,2-Tetrachloroeth...	10.213	84	237932	39.016	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	78.040%
66) 1,2-Dichlorobenzene-d4	11.622	152	170031	50.314	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	100.620%
Target Compounds						
39) cis-1,3-Dichloropropene	6.982	75	4818	0.921	ug/L	# 45


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081022\
Data File : VV027253.D
Acq On : 10 Aug 2022 12:11
Operator : SY/MD
Sample : VV0810WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK257

Quant Time: Aug 11 03:53:31 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Aug 09 02:29:12 2022
Response via : Initial Calibration

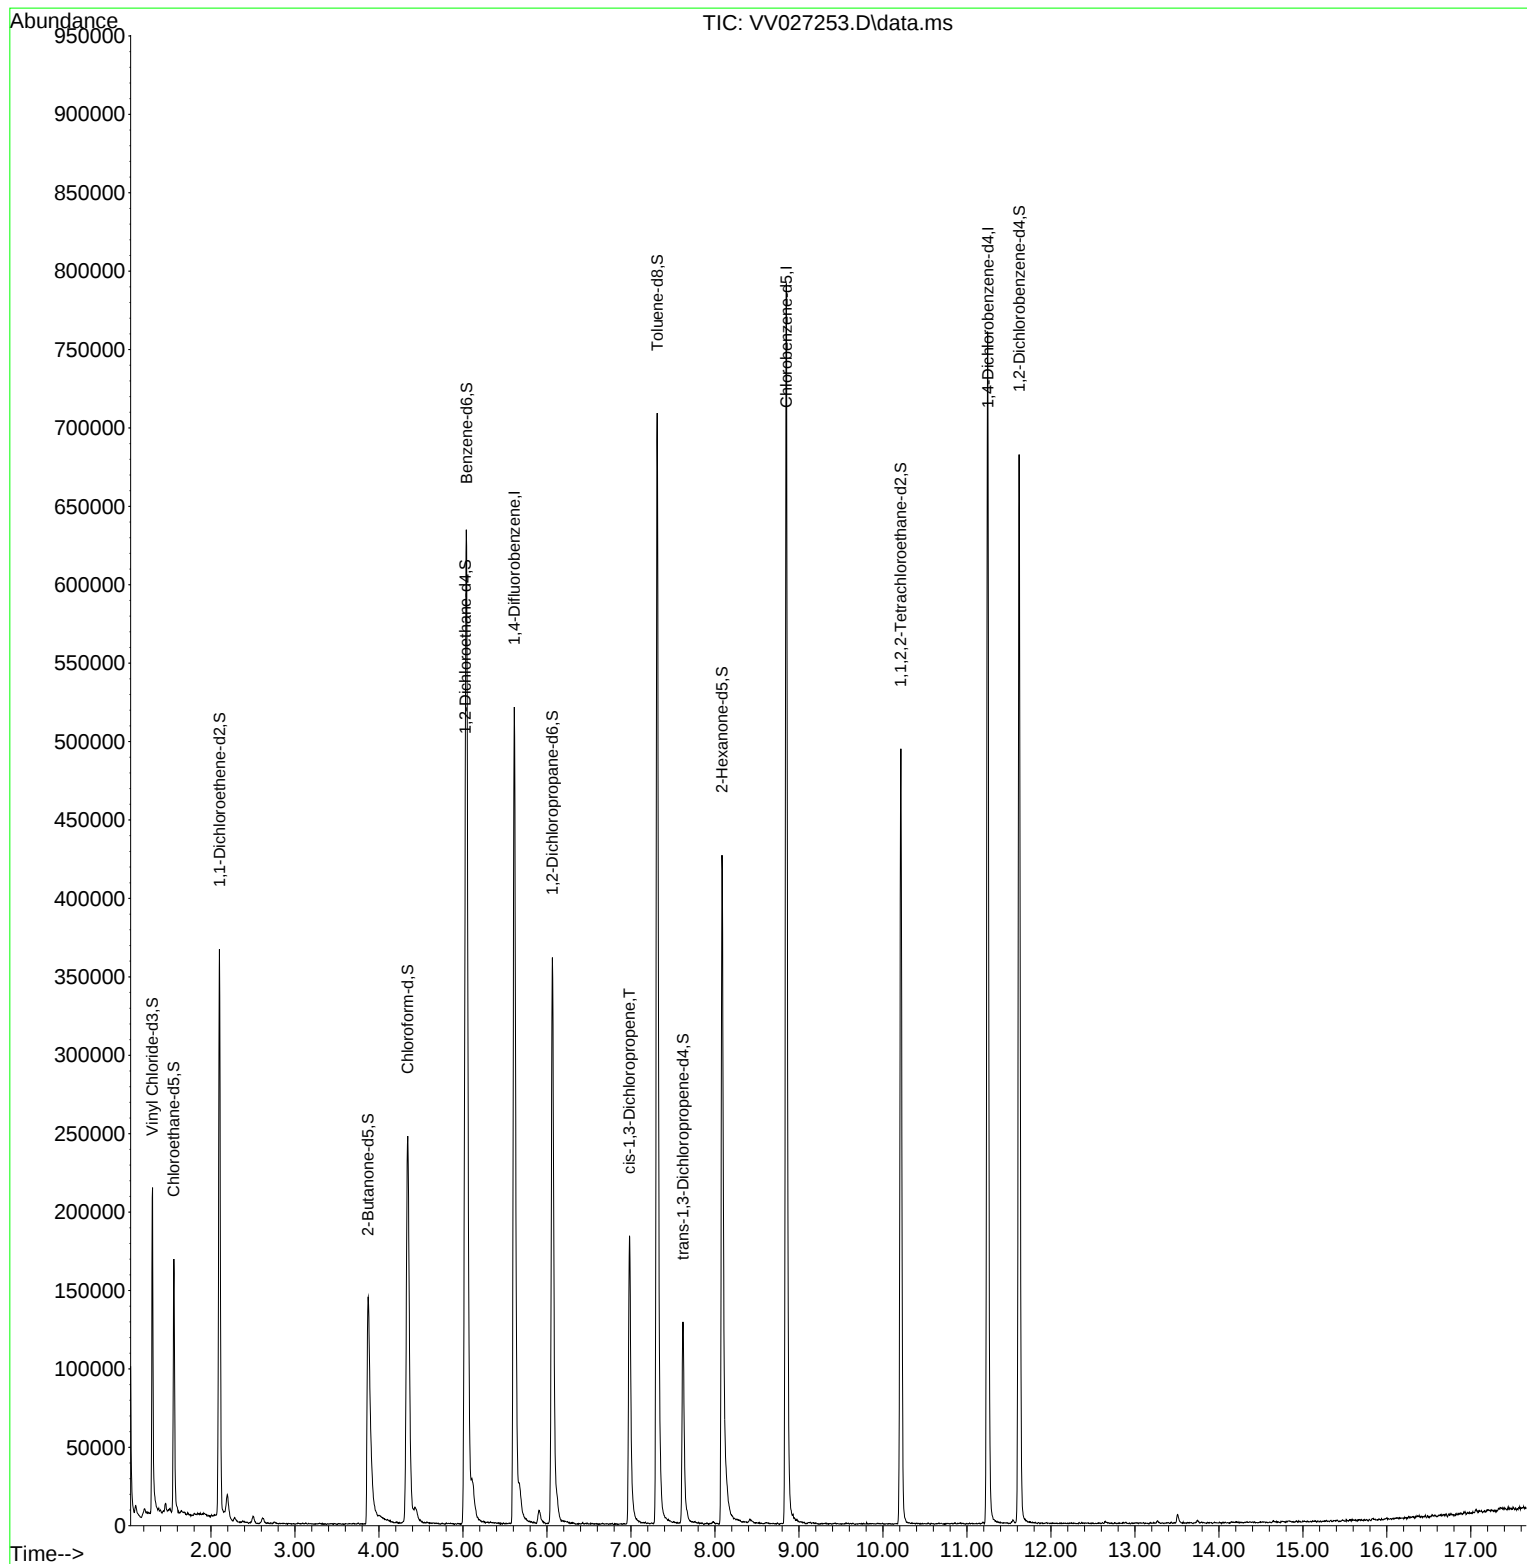

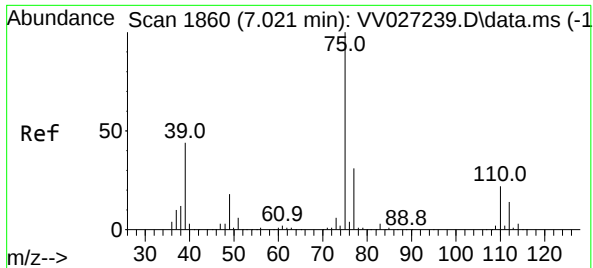

#39
 cis-1,3-Dichloropropene
 Concen: 0.921 ug/L
 RT: 6.982 min Scan# 11
 Delta R.T. -0.039 min
 Lab File: VV027253.D
 Acq: 10 Aug 2022 12:11

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK257

Tgt Ion: 75 Resp: 4818
 Ion Ratio Lower Upper
 75 100
 77 62.8 22.5 41.7#

