

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081022\
 Data File : VV027252.D
 Acq On : 10 Aug 2022 11:53
 Operator : SY/MD
 Sample : VV0810MBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK256

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

Signal : TIC: VV027252.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	74	81	101	rBV	211466	228807	13.72%	1.803%
2	1.555	153	160	178	rVB	164731	197116	11.82%	1.553%
3	2.095	319	328	342	rBV	357201	511011	30.65%	4.027%
4	2.561	471	473	477	rBV4	519	318	0.02%	0.003%
5	2.677	507	509	512	rBV3	524	315	0.02%	0.002%
6	2.754	525	533	537	rBV6	1994	2575	0.15%	0.020%
7	2.825	553	555	559	rVB4	668	367	0.02%	0.003%
8	2.850	561	563	566	rBV3	398	255	0.02%	0.002%
9	2.976	598	602	607	rBV3	624	577	0.03%	0.005%
10	3.092	634	638	642	rVB3	573	528	0.03%	0.004%
11	3.117	642	646	647	rBV3	725	470	0.03%	0.004%
12	3.204	671	673	679	rVB3	1010	745	0.04%	0.006%
13	3.526	769	773	775	rBV2	430	278	0.02%	0.002%
14	3.632	802	806	808	rBV2	311	245	0.01%	0.002%
15	3.645	808	810	814	rVB2	587	266	0.02%	0.002%
16	3.674	816	819	821	rVV3	497	257	0.02%	0.002%
17	3.686	821	823	826	rVB2	611	270	0.02%	0.002%
18	3.744	835	841	845	rBV4	504	649	0.04%	0.005%
19	3.863	868	878	910	rBV	134287	368886	22.12%	2.907%
20	4.166	967	972	982	rBV9	1510	2165	0.13%	0.017%
21	4.336	1011	1025	1049	rBV	245824	614438	36.85%	4.842%
22	4.567	1094	1097	1101	rVB3	1054	681	0.04%	0.005%
23	4.786	1163	1165	1167	rBV	498	204	0.01%	0.002%
24	4.802	1167	1170	1177	rBV4	568	616	0.04%	0.005%
25	4.834	1177	1180	1183	rVB2	796	525	0.03%	0.004%
26	4.883	1193	1195	1200	rVB2	510	213	0.01%	0.002%
27	4.915	1201	1205	1207	rBV3	358	219	0.01%	0.002%
28	4.928	1207	1209	1213	rVB2	578	380	0.02%	0.003%
29	4.950	1213	1216	1220	rBV3	609	410	0.02%	0.003%
30	4.969	1220	1222	1225	rBV2	377	239	0.01%	0.002%
31	5.034	1225	1242	1284	rBV2	628060	1667383	100.00%	13.139%
32	5.606	1408	1420	1457	rBV	519642	1084355	65.03%	8.545%
33	5.847	1493	1495	1497	rBV3	583	306	0.02%	0.002%
34	5.905	1502	1513	1522	rVV8	8270	16445	0.99%	0.130%
35	6.059	1547	1561	1590	rBV	353316	759137	45.53%	5.982%
36	6.346	1649	1650	1652	rVB2	619	203	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081022\
 Data File : VV027252.D
 Acq On : 10 Aug 2022 11:53
 Operator : SY/MD
 Sample : VV0810MBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK256

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

37	6.362	1652	1655	1656	rBV2	727	518	0.03%	0.004%
38	6.497	1694	1697	1698	rBV2	880	374	0.02%	0.003%
39	6.506	1698	1700	1702	rBV2	436	241	0.01%	0.002%
40	6.625	1735	1737	1740	rBV2	798	359	0.02%	0.003%
41	6.654	1744	1746	1749	rVB3	662	269	0.02%	0.002%
42	6.673	1749	1752	1755	rBV3	320	293	0.02%	0.002%
43	6.892	1816	1820	1823	rBV3	589	467	0.03%	0.004%
44	6.911	1823	1826	1830	rVB3	614	506	0.03%	0.004%
45	6.979	1834	1847	1876	rBV	187277	363988	21.83%	2.868%
46	7.165	1902	1905	1906	rBV	458	233	0.01%	0.002%
47	7.188	1910	1912	1914	rBV2	413	226	0.01%	0.002%
48	7.310	1938	1950	1983	rBV	721637	1296501	77.76%	10.216%
49	7.551	2022	2025	2026	rBV3	527	304	0.02%	0.002%
50	7.616	2035	2045	2074	rBV	130117	240995	14.45%	1.899%
51	7.902	2130	2134	2136	rBV3	676	473	0.03%	0.004%
52	7.969	2153	2155	2160	rBV4	871	769	0.05%	0.006%
53	8.085	2180	2191	2227	rBV	403507	784527	47.05%	6.182%
54	8.606	2349	2353	2357	rBV3	1015	823	0.05%	0.006%
55	8.673	2371	2374	2376	rBV3	725	550	0.03%	0.004%
56	8.709	2383	2385	2390	rVB2	642	326	0.02%	0.003%
57	8.754	2395	2399	2400	rBV3	431	277	0.02%	0.002%
58	8.847	2417	2428	2455	rBV	796000	1317558	79.02%	10.382%
59	9.104	2506	2508	2510	rBV3	679	316	0.02%	0.002%
60	9.143	2517	2520	2523	rBV3	1090	807	0.05%	0.006%
61	9.191	2532	2535	2537	rBV2	481	354	0.02%	0.003%
62	9.239	2548	2550	2555	rVB4	575	400	0.02%	0.003%
63	9.265	2555	2558	2561	rBV3	427	332	0.02%	0.003%
64	9.435	2607	2611	2612	rBV3	555	360	0.02%	0.003%
65	9.542	2641	2644	2645	rBV2	722	390	0.02%	0.003%
66	9.779	2714	2718	2721	rBV	533	598	0.04%	0.005%
67	9.812	2725	2728	2730	rBV2	645	436	0.03%	0.003%
68	9.844	2733	2738	2741	rBV2	605	457	0.03%	0.004%
69	9.898	2751	2755	2759	rBV2	522	440	0.03%	0.003%
70	9.927	2759	2764	2765	rBV3	1016	774	0.05%	0.006%
71	9.998	2783	2786	2790	rVB2	533	402	0.02%	0.003%
72	10.024	2791	2794	2796	rBV	438	312	0.02%	0.002%
73	10.098	2814	2817	2819	rBV	391	234	0.01%	0.002%
74	10.159	2834	2836	2840	rVB2	373	261	0.02%	0.002%
75	10.214	2841	2853	2881	rVB	488697	774113	46.43%	6.100%
76	10.374	2901	2903	2905	rBV2	526	326	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081022\
 Data File : VV027252.D
 Acq On : 10 Aug 2022 11:53
 Operator : SY/MD
 Sample : VV0810MBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK256

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

77	10.406	2911	2913	2917	rVB2	579	302	0.02%	0.002%
78	10.429	2917	2920	2922	rBV2	634	441	0.03%	0.003%
79	10.445	2922	2925	2927	rVV2	501	283	0.02%	0.002%
80	10.609	2974	2976	2979	rBV3	478	251	0.02%	0.002%
81	10.834	3040	3046	3047	rBV3	734	562	0.03%	0.004%
82	10.914	3067	3071	3073	rBV3	1282	1117	0.07%	0.009%
83	11.085	3120	3124	3127	rBV3	597	457	0.03%	0.004%
84	11.104	3127	3130	3134	rVB5	595	437	0.03%	0.003%
85	11.123	3134	3136	3140	rVB3	707	385	0.02%	0.003%
86	11.149	3141	3144	3146	rBV3	416	302	0.02%	0.002%
87	11.181	3150	3154	3159	rBV5	2289	2815	0.17%	0.022%
88	11.246	3163	3174	3201	rVV	794176	1234241	74.02%	9.726%
89	11.484	3243	3248	3251	rBV3	812	731	0.04%	0.006%
90	11.622	3279	3291	3313	rBV	720350	1119614	67.15%	8.822%
91	12.644	3604	3609	3620	rVB9	4444	7160	0.43%	0.056%
92	12.728	3633	3635	3638	rVB	554	246	0.01%	0.002%
93	12.744	3638	3640	3643	rVB	664	271	0.02%	0.002%
94	12.770	3644	3648	3651	rBV2	526	292	0.02%	0.002%
95	12.879	3680	3682	3683	rBV	642	247	0.01%	0.002%
96	12.969	3707	3710	3712	rBV	752	383	0.02%	0.003%
97	13.265	3795	3802	3812	rVB7	6402	9711	0.58%	0.077%
98	13.503	3868	3876	3892	rBV	25200	42318	2.54%	0.333%
99	13.747	3944	3952	3963	rVB5	8539	13390	0.80%	0.106%
100	14.635	4225	4228	4230	rBV3	1140	853	0.05%	0.007%




Sum of corrected areas: 12690552

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081022\
Data File : VV027252.D
Acq On : 10 Aug 2022 11:53
Operator : SY/MD
Sample : VV0810MBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK256

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

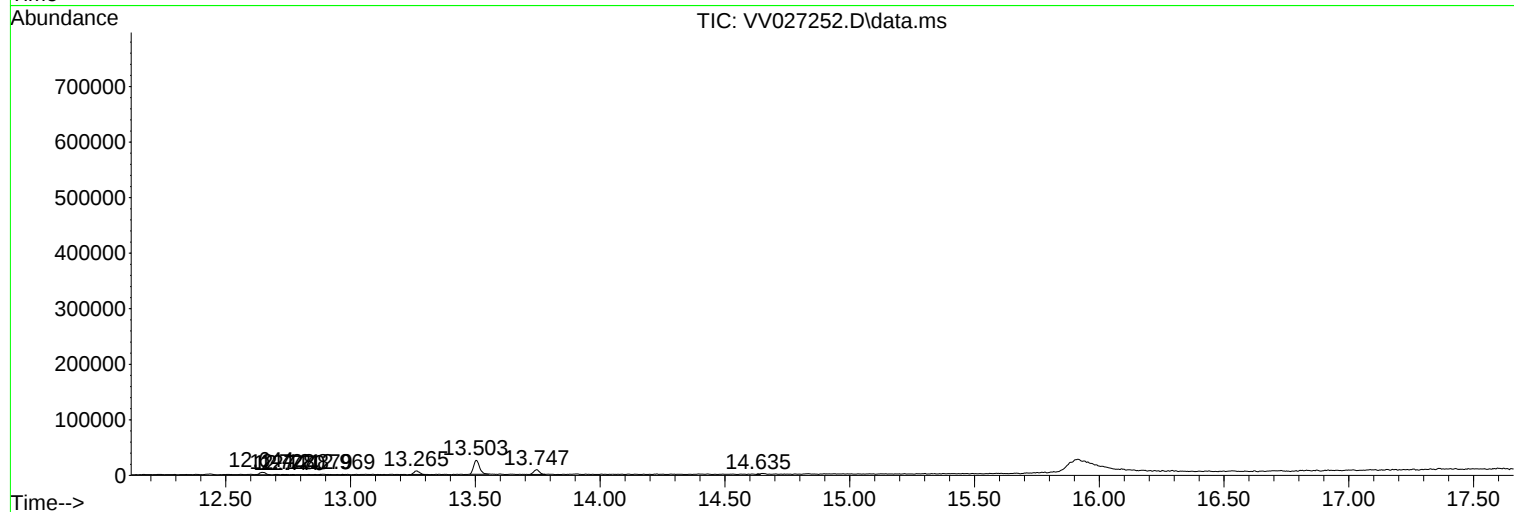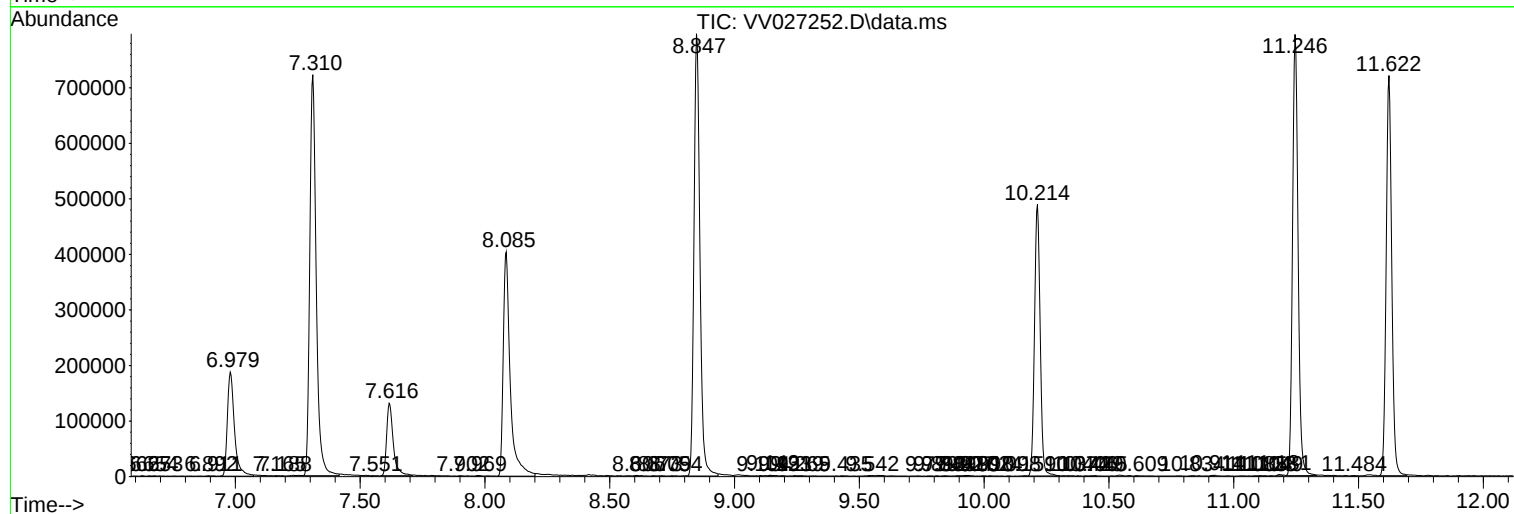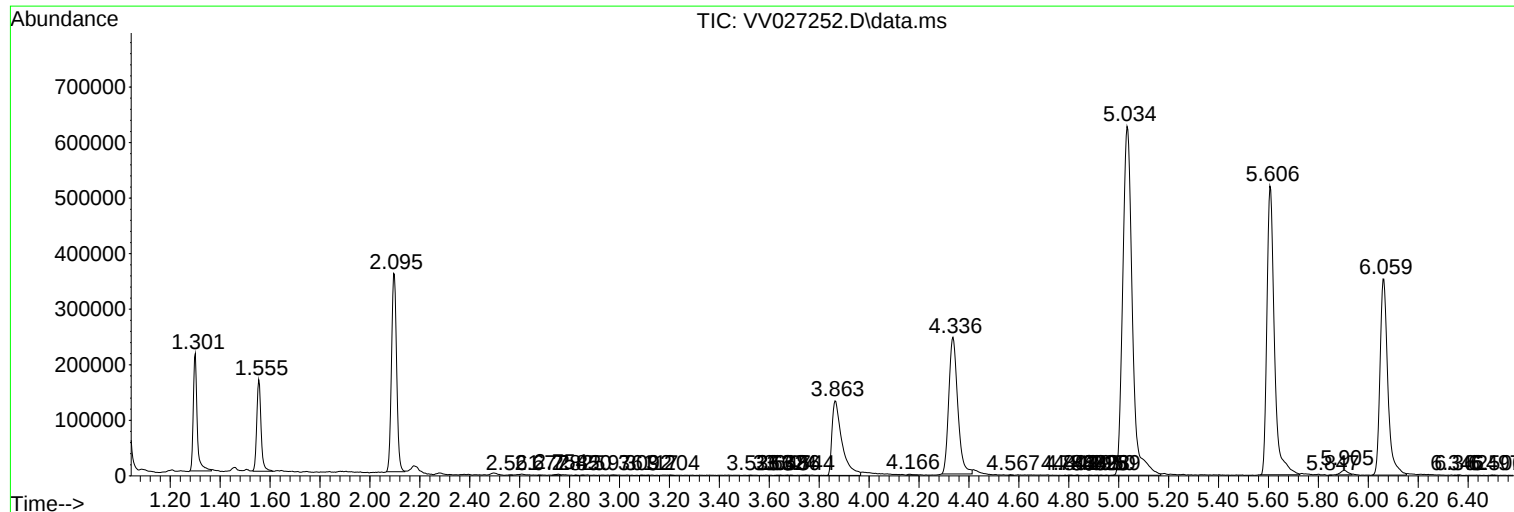

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081022\
Data File : VV027252.D
Acq On : 10 Aug 2022 11:53
Operator : SY/MD
Sample : VV0810MBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK256

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081022\
Data File : VV027252.D
Acq On : 10 Aug 2022 11:53
Operator : SY/MD
Sample : VV0810MBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK256

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc