

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081022\
 Data File : VV027253.D
 Acq On : 10 Aug 2022 12:11
 Operator : SY/MD
 Sample : VV0810WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK257

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

Signal : TIC: VV027253.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	101	rBV	207310	226109	14.09%	1.803%
2	1.558	155	161	177	rVB	161770	193344	12.05%	1.541%
3	2.101	321	330	345	rVB	358907	502898	31.34%	4.010%
4	2.735	525	527	529	rBV	611	339	0.02%	0.003%
5	2.918	581	584	587	rBV2	737	654	0.04%	0.005%
6	2.979	598	603	605	rBV2	538	519	0.03%	0.004%
7	3.034	618	620	623	rBV2	633	366	0.02%	0.003%
8	3.239	680	684	686	rVB2	237	177	0.01%	0.001%
9	3.252	686	688	692	rBV3	428	331	0.02%	0.003%
10	3.323	709	710	713	rBV	478	141	0.01%	0.001%
11	3.336	713	714	717	rVB2	522	225	0.01%	0.002%
12	3.362	717	722	726	rVB2	471	398	0.02%	0.003%
13	3.391	726	731	735	rBV4	439	483	0.03%	0.004%
14	3.465	752	754	755	rBV	663	244	0.02%	0.002%
15	3.516	768	770	773	rBV3	583	496	0.03%	0.004%
16	3.600	791	796	797	rBV2	553	414	0.03%	0.003%
17	3.683	821	822	824	rBV	388	207	0.01%	0.002%
18	3.748	839	842	844	rBV2	518	407	0.03%	0.003%
19	3.780	849	852	855	rBV2	366	291	0.02%	0.002%
20	3.828	865	867	870	rVB2	383	179	0.01%	0.001%
21	3.873	871	881	916	rBV	144832	416529	25.96%	3.321%
22	4.265	1001	1003	1006	rBV2	503	353	0.02%	0.003%
23	4.342	1012	1027	1050	rBV2	245671	624274	38.91%	4.977%
24	4.744	1148	1152	1154	rBV2	632	468	0.03%	0.004%
25	4.802	1167	1170	1174	rBV3	822	576	0.04%	0.005%
26	4.905	1200	1202	1208	rBV2	543	513	0.03%	0.004%
27	4.940	1208	1213	1215	rBV3	593	489	0.03%	0.004%
28	5.040	1224	1244	1262	rBV2	634245	1604450	100.00%	12.792%
29	5.448	1370	1371	1372	rBV2	676	220	0.01%	0.002%
30	5.503	1386	1388	1389	rBV2	395	130	0.01%	0.001%
31	5.612	1410	1422	1438	rBV	520567	1052589	65.60%	8.392%
32	5.905	1504	1513	1531	rBV6	8441	19749	1.23%	0.157%
33	6.066	1550	1563	1596	rBV	360235	759768	47.35%	6.057%
34	6.355	1650	1653	1657	rBV4	307	241	0.02%	0.002%
35	6.371	1657	1658	1659	rBV	320	83	0.01%	0.001%
36	6.426	1669	1675	1680	rVB4	1190	1153	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081022\
 Data File : VV027253.D
 Acq On : 10 Aug 2022 12:11
 Operator : SY/MD
 Sample : VV0810WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK257

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

37	6.452	1680	1683	1684	rBV	453	312	0.02%	0.002%
38	6.477	1689	1691	1695	rVB3	623	474	0.03%	0.004%
39	6.522	1703	1705	1708	rBV	809	379	0.02%	0.003%
40	6.554	1713	1715	1718	rVB3	390	176	0.01%	0.001%
41	6.571	1718	1720	1722	rBV2	341	182	0.01%	0.001%
42	6.622	1734	1736	1740	rBV4	595	472	0.03%	0.004%
43	6.651	1741	1745	1746	rBV2	292	187	0.01%	0.001%
44	6.747	1770	1775	1776	rBV2	415	341	0.02%	0.003%
45	6.805	1791	1793	1794	rBV	437	139	0.01%	0.001%
46	6.831	1799	1801	1806	rVB2	615	371	0.02%	0.003%
47	6.853	1806	1808	1809	rBV	266	135	0.01%	0.001%
48	6.889	1817	1819	1821	rVB2	378	160	0.01%	0.001%
49	6.915	1823	1827	1828	rBV2	406	254	0.02%	0.002%
50	6.982	1836	1848	1873	rBV	183845	355684	22.17%	2.836%
51	7.313	1939	1951	1980	rBV	707696	1283605	80.00%	10.234%
52	7.619	2037	2046	2078	rVB	127642	234542	14.62%	1.870%
53	7.879	2124	2127	2129	rBV2	690	464	0.03%	0.004%
54	7.934	2142	2144	2146	rBV2	488	214	0.01%	0.002%
55	8.085	2180	2191	2226	rBV	426657	831414	51.82%	6.629%
56	8.529	2328	2329	2332	rVB3	733	272	0.02%	0.002%
57	8.773	2403	2405	2406	rBV	299	159	0.01%	0.001%
58	8.850	2417	2429	2451	rBV	790567	1331033	82.96%	10.612%
59	9.111	2507	2510	2512	rBV3	787	611	0.04%	0.005%
60	9.197	2536	2537	2539	rBV2	521	237	0.01%	0.002%
61	9.236	2547	2549	2551	rVB2	413	148	0.01%	0.001%
62	9.268	2556	2559	2560	rBV	496	271	0.02%	0.002%
63	9.336	2578	2580	2583	rVB2	367	133	0.01%	0.001%
64	9.358	2586	2587	2590	rBV2	512	303	0.02%	0.002%
65	9.406	2598	2602	2604	rBV2	612	444	0.03%	0.004%
66	9.554	2645	2648	2650	rBV3	644	358	0.02%	0.003%
67	9.612	2662	2666	2667	rBV3	573	344	0.02%	0.003%
68	9.677	2684	2686	2688	rBV2	453	256	0.02%	0.002%
69	9.747	2707	2708	2710	rBV2	423	147	0.01%	0.001%
70	9.805	2724	2726	2727	rBV	761	165	0.01%	0.001%
71	9.831	2732	2734	2735	rBV	306	99	0.01%	0.001%
72	10.062	2804	2806	2808	rBV2	349	154	0.01%	0.001%
73	10.133	2826	2828	2829	rBV2	263	123	0.01%	0.001%
74	10.213	2840	2853	2874	rBV	494306	782061	48.74%	6.235%
75	10.442	2923	2924	2927	rBV	363	194	0.01%	0.002%
76	10.471	2931	2933	2936	rVB	443	177	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081022\
 Data File : VV027253.D
 Acq On : 10 Aug 2022 12:11
 Operator : SY/MD
 Sample : VV0810WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK257

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

77	10.538	2952	2954	2962	rVB4	1026	969	0.06%	0.008%
78	10.574	2962	2965	2967	rBV2	861	580	0.04%	0.005%
79	10.738	3014	3016	3017	rBV2	350	100	0.01%	0.001%
80	10.747	3017	3019	3020	rBV2	231	100	0.01%	0.001%
81	10.754	3020	3021	3024	rBV3	399	205	0.01%	0.002%
82	10.853	3046	3052	3054	rBV4	842	790	0.05%	0.006%
83	10.892	3062	3064	3067	rBV3	557	316	0.02%	0.003%
84	10.988	3092	3094	3095	rBV3	321	119	0.01%	0.001%
85	11.246	3162	3174	3196	rBV	760321	1209797	75.40%	9.645%
86	11.622	3280	3291	3315	rBV	679924	1079506	67.28%	8.607%
87	12.127	3446	3448	3451	rBV2	622	359	0.02%	0.003%
88	12.268	3490	3492	3495	rBV2	443	177	0.01%	0.001%
89	12.336	3510	3513	3519	rBV2	803	671	0.04%	0.005%
90	12.647	3606	3610	3613	rBV4	1296	1153	0.07%	0.009%
91	12.934	3697	3699	3703	rVB3	762	430	0.03%	0.003%
92	12.963	3704	3708	3710	rBV2	705	578	0.04%	0.005%
93	13.181	3774	3776	3777	rBV	698	292	0.02%	0.002%
94	13.509	3872	3878	3891	rVB5	5447	9245	0.58%	0.074%
95	13.573	3896	3898	3899	rBV2	768	218	0.01%	0.002%




Sum of corrected areas: 12542606

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081022\
Data File : VV027253.D
Acq On : 10 Aug 2022 12:11
Operator : SY/MD
Sample : VV0810WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK257

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

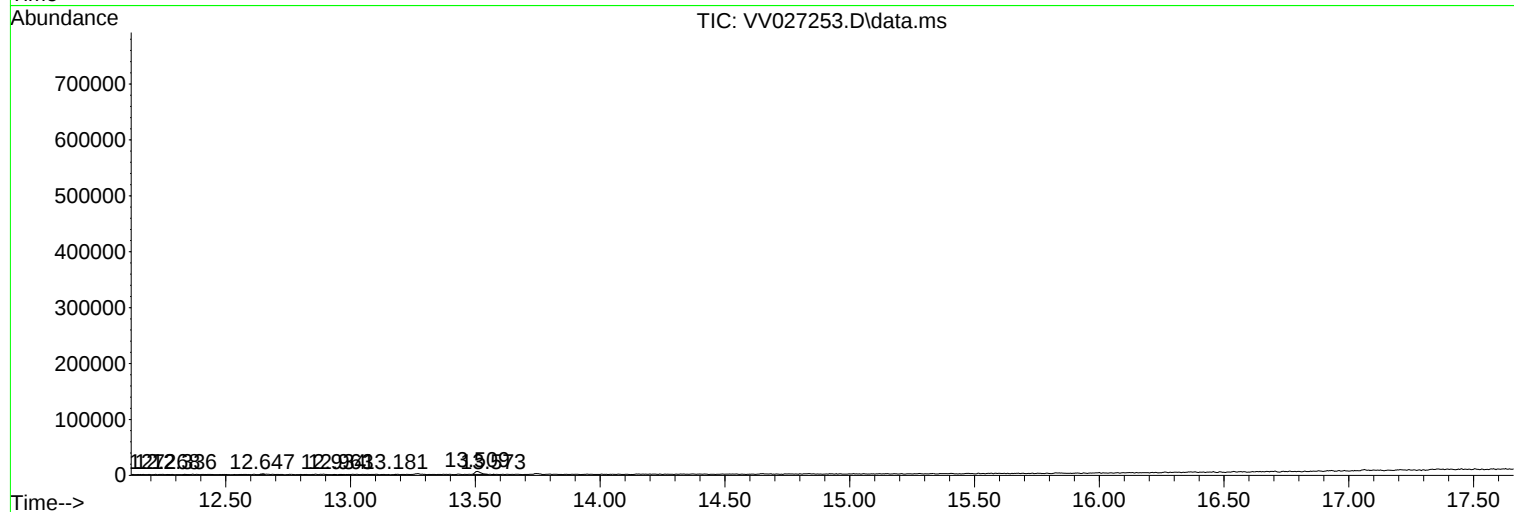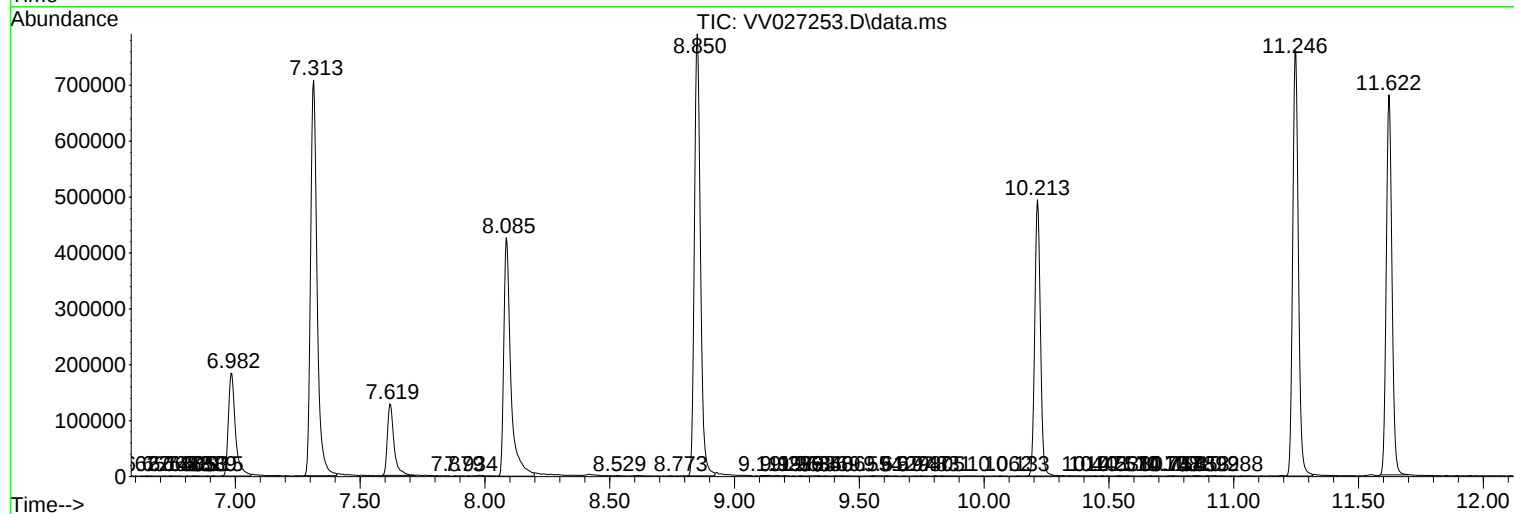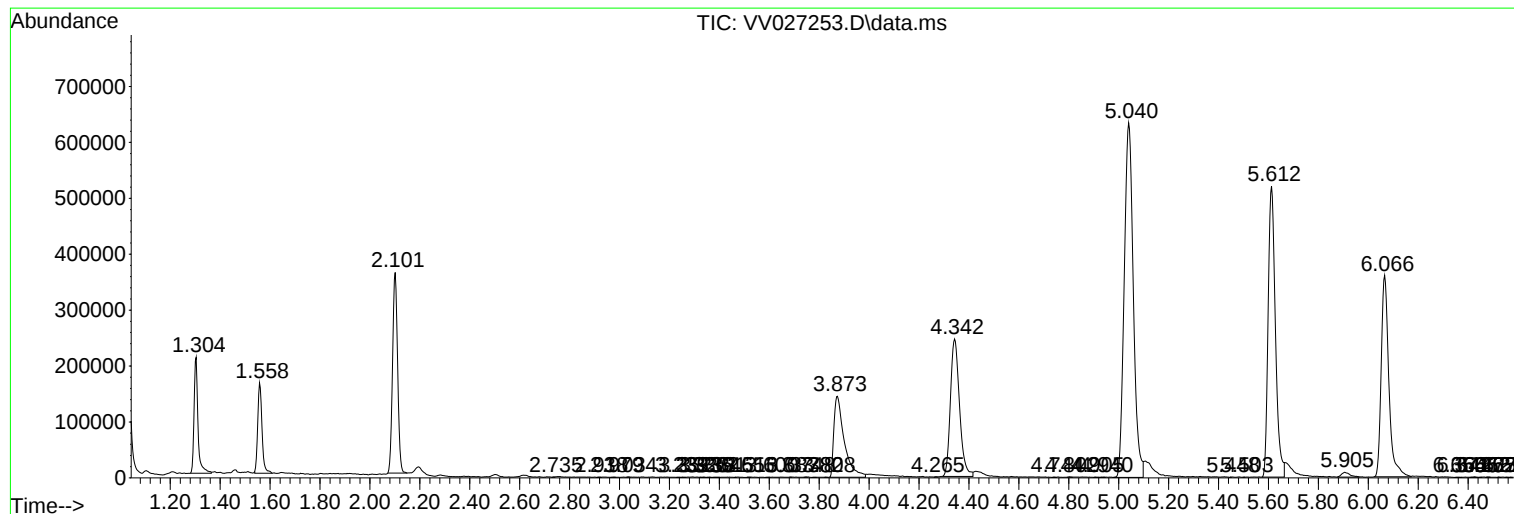

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081022\
Data File : VV027253.D
Acq On : 10 Aug 2022 12:11
Operator : SY/MD
Sample : VV0810WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK257

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081022\
Data File : VV027253.D
Acq On : 10 Aug 2022 12:11
Operator : SY/MD
Sample : VV0810WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK257

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc