

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081022\
 Data File : VV027259.D
 Acq On : 10 Aug 2022 15:51
 Operator : SY/MD
 Sample : N4114-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E28

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

Signal : TIC: VV027259.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	74	81	89	rBV2	233225	254377	15.17%	1.913%
2	1.558	155	161	179	rVB	166113	197094	11.75%	1.482%
3	2.098	321	329	342	rVB	331228	463807	27.66%	3.487%
4	2.751	526	532	533	rBV4	3305	3203	0.19%	0.024%
5	3.021	613	616	617	rBV2	565	266	0.02%	0.002%
6	3.150	654	656	657	rBV	663	255	0.02%	0.002%
7	3.281	694	697	699	rBV3	532	312	0.02%	0.002%
8	3.294	699	701	706	rVV4	429	289	0.02%	0.002%
9	3.510	764	768	772	rVB4	777	748	0.04%	0.006%
10	3.535	772	776	777	rBV	274	182	0.01%	0.001%
11	3.645	808	810	813	rVB	320	161	0.01%	0.001%
12	3.661	813	815	816	rBV	462	186	0.01%	0.001%
13	3.751	839	843	844	rBV2	453	282	0.02%	0.002%
14	3.783	849	853	856	rVV4	640	605	0.04%	0.005%
15	3.799	856	858	862	rVB	417	229	0.01%	0.002%
16	3.899	870	889	915	rBV2	254559	961440	57.34%	7.229%
17	4.342	1009	1027	1048	rBV	270284	677923	40.43%	5.097%
18	4.709	1139	1141	1143	rVB3	531	198	0.01%	0.001%
19	4.815	1171	1174	1177	rBV2	703	435	0.03%	0.003%
20	4.860	1183	1188	1190	rBV3	452	403	0.02%	0.003%
21	4.912	1202	1204	1205	rBV	405	186	0.01%	0.001%
22	4.957	1216	1218	1219	rBV	390	145	0.01%	0.001%
23	5.040	1228	1244	1263	rBV2	655435	1676814	100.00%	12.608%
24	5.465	1374	1376	1379	rVB3	847	284	0.02%	0.002%
25	5.503	1383	1388	1392	rBV3	831	825	0.05%	0.006%
26	5.545	1399	1401	1403	rBV2	704	283	0.02%	0.002%
27	5.612	1410	1422	1457	rBV	459770	977461	58.29%	7.349%
28	6.066	1547	1563	1597	rBV	390627	827406	49.34%	6.221%
29	6.461	1684	1686	1689	rBV2	443	288	0.02%	0.002%
30	6.510	1697	1701	1704	rBV5	620	516	0.03%	0.004%
31	6.542	1709	1711	1715	rVB3	564	329	0.02%	0.002%
32	6.567	1715	1719	1722	rBV3	701	606	0.04%	0.005%
33	6.628	1729	1738	1741	rBV6	910	1177	0.07%	0.009%
34	6.844	1803	1805	1806	rBV6	249	128	0.01%	0.001%
35	6.850	1806	1807	1810	rVB2	451	184	0.01%	0.001%
36	6.870	1811	1813	1815	rVB2	493	184	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081022\
 Data File : VV027259.D
 Acq On : 10 Aug 2022 15:51
 Operator : SY/MD
 Sample : N4114-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E28

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

37	6.908	1822	1825	1827	rBV2	385	314	0.02%	0.002%
38	6.982	1837	1848	1876	rBV	189643	365509	21.80%	2.748%
39	7.198	1912	1915	1917	rBV3	770	548	0.03%	0.004%
40	7.313	1939	1951	1973	rBV	698461	1256846	74.95%	9.450%
41	7.619	2037	2046	2075	rBV	133908	244965	14.61%	1.842%
42	7.937	2142	2145	2147	rBV	451	324	0.02%	0.002%
43	8.085	2181	2191	2226	rBV	528601	1004830	59.92%	7.555%
44	8.667	2370	2372	2375	rBV2	654	250	0.01%	0.002%
45	8.735	2390	2393	2395	rBV4	717	390	0.02%	0.003%
46	8.776	2402	2406	2410	rBV4	563	583	0.03%	0.004%
47	8.850	2418	2429	2454	rBV	727917	1200636	71.60%	9.027%
48	9.149	2521	2522	2524	rBV2	854	394	0.02%	0.003%
49	9.252	2551	2554	2555	rBV2	281	133	0.01%	0.001%
50	9.339	2579	2581	2586	rVB5	553	439	0.03%	0.003%
51	9.464	2616	2620	2621	rBV2	589	442	0.03%	0.003%
52	9.497	2626	2630	2631	rBV	731	464	0.03%	0.003%
53	9.548	2644	2646	2648	rBV3	628	225	0.01%	0.002%
54	9.587	2657	2658	2660	rVB	661	160	0.01%	0.001%
55	9.644	2674	2676	2678	rBV3	388	217	0.01%	0.002%
56	9.767	2711	2714	2717	rVB2	825	453	0.03%	0.003%
57	9.792	2717	2722	2727	rVB3	1096	870	0.05%	0.007%
58	9.821	2727	2731	2734	rBV3	800	617	0.04%	0.005%
59	9.850	2734	2740	2743	rBV4	702	795	0.05%	0.006%
60	9.972	2776	2778	2780	rBV4	424	177	0.01%	0.001%
61	9.992	2782	2784	2785	rBV	242	102	0.01%	0.001%
62	10.005	2785	2788	2792	rVV3	713	451	0.03%	0.003%
63	10.104	2816	2819	2821	rBV	654	426	0.03%	0.003%
64	10.169	2837	2839	2840	rBV	664	232	0.01%	0.002%
65	10.214	2841	2853	2877	rVV	575032	925373	55.19%	6.958%
66	10.387	2905	2907	2910	rVB4	593	329	0.02%	0.002%
67	10.638	2984	2985	2987	rBV	280	90	0.01%	0.001%
68	10.853	3049	3052	3055	rBV5	992	751	0.04%	0.006%
69	10.924	3072	3074	3076	rBV3	888	486	0.03%	0.004%
70	10.956	3081	3084	3088	rBV4	565	469	0.03%	0.004%
71	10.976	3088	3090	3094	rBV2	437	298	0.02%	0.002%
72	11.123	3133	3136	3139	rVB4	659	398	0.02%	0.003%
73	11.143	3139	3142	3143	rBV2	579	250	0.01%	0.002%
74	11.249	3163	3175	3198	rBV	690489	1061494	63.30%	7.981%
75	11.435	3230	3233	3234	rBV2	685	382	0.02%	0.003%
76	11.545	3261	3267	3268	rBV3	1618	1676	0.10%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081022\
Data File : VV027259.D
Acq On : 10 Aug 2022 15:51
Operator : SY/MD
Sample : N4114-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E28

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M

Title : VOC Analysis

77	11.622	3279	3291	3314	rBV	743623	1174494	70.04%	8.831%
78	12.011	3410	3412	3416	rBV3	718	427	0.03%	0.003%
79	12.111	3441	3443	3447	rVB2	828	472	0.03%	0.004%
80	12.143	3447	3453	3455	rBV3	745	666	0.04%	0.005%
81	12.493	3559	3562	3565	rBV2	767	478	0.03%	0.004%
82	13.316	3816	3818	3823	rBV2	574	483	0.03%	0.004%




Sum of corrected areas: 13300019

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081022\
Data File : VV027259.D
Acq On : 10 Aug 2022 15:51
Operator : SY/MD
Sample : N4114-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E28

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

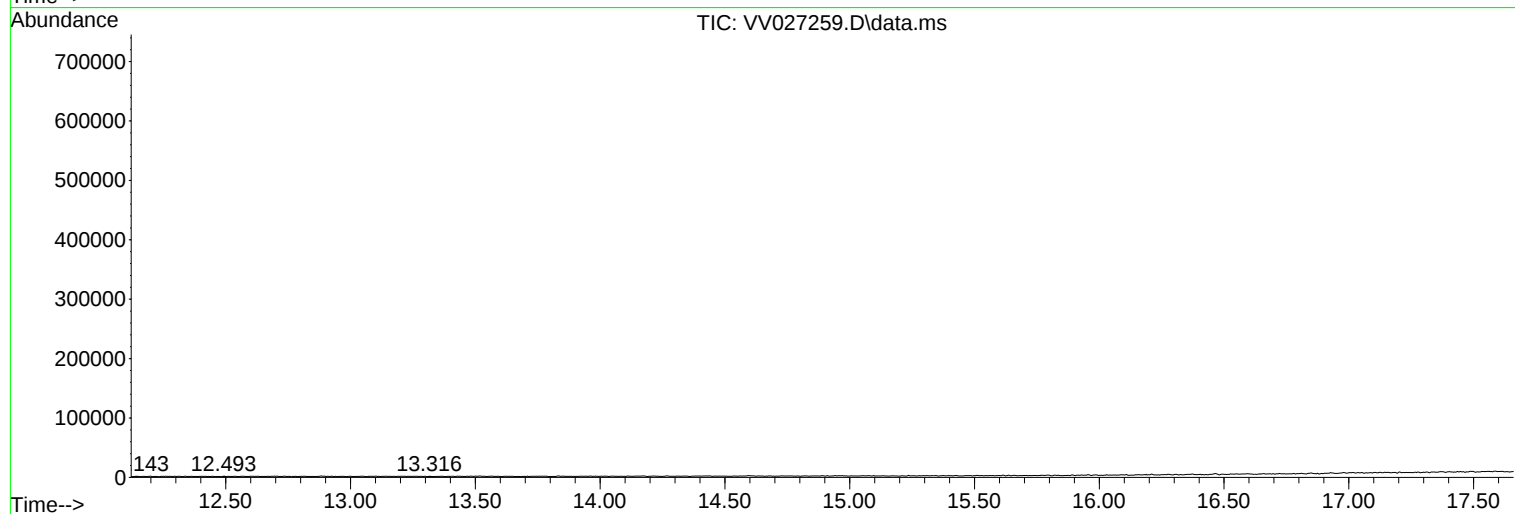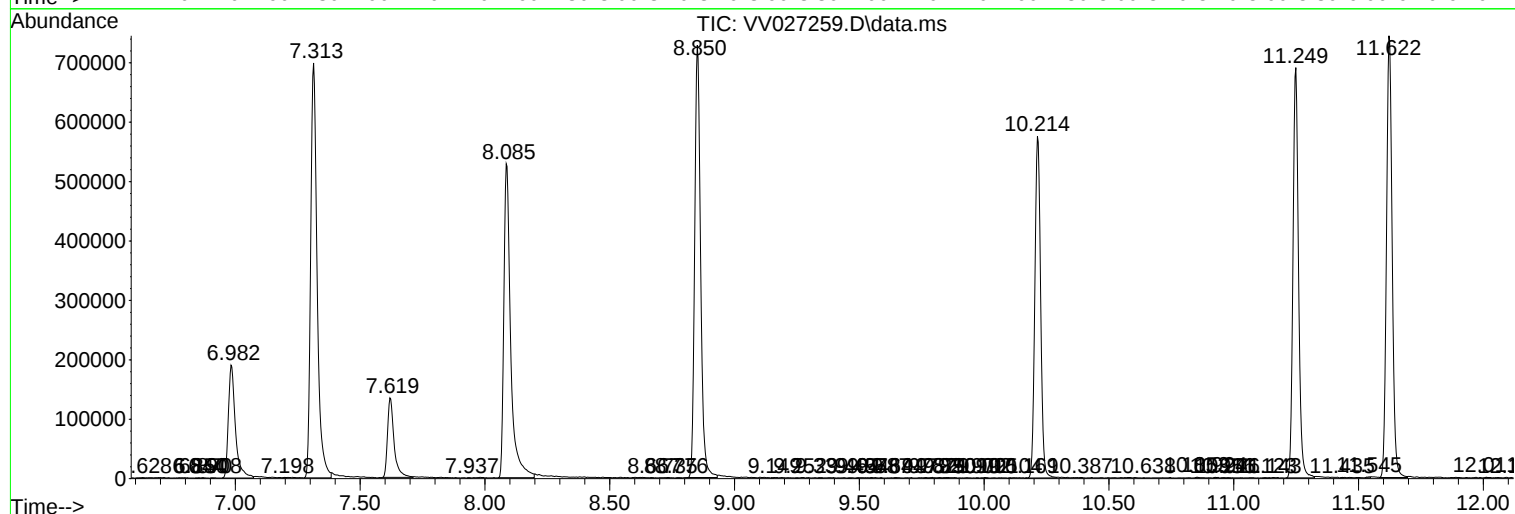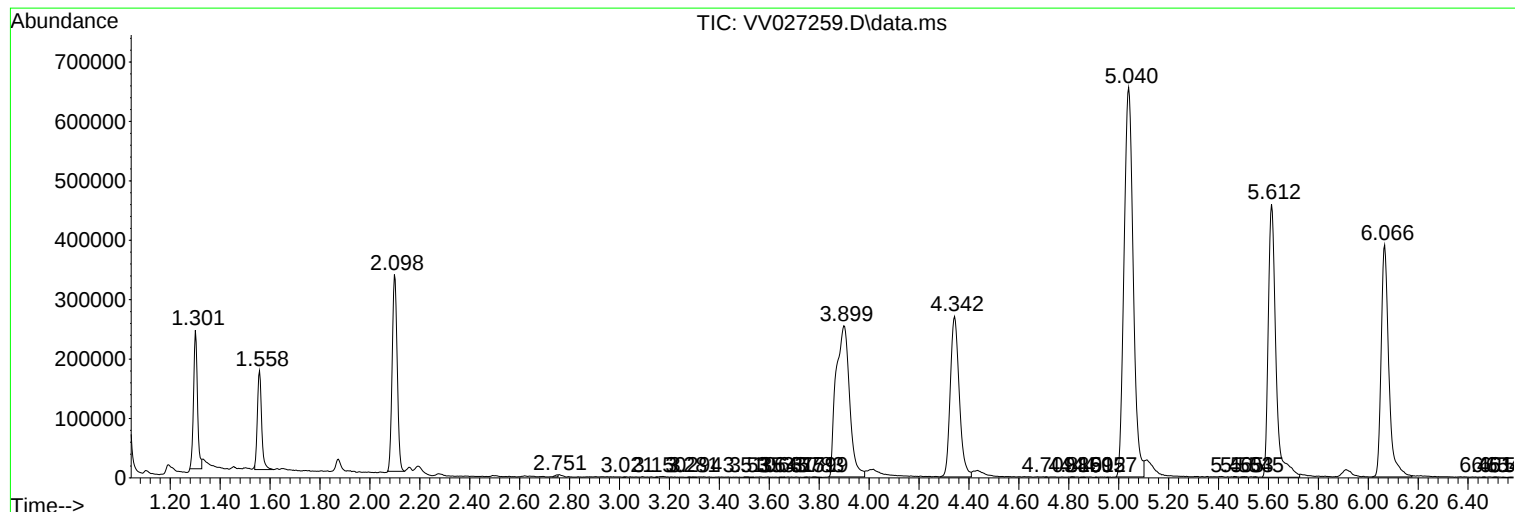

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081022\
Data File : VV027259.D
Acq On : 10 Aug 2022 15:51
Operator : SY/MD
Sample : N4114-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E28

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081022\
Data File : VV027259.D
Acq On : 10 Aug 2022 15:51
Operator : SY/MD
Sample : N4114-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E28

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc