

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081022\
 Data File : VV027261.D
 Acq On : 10 Aug 2022 16:41
 Operator : SY/MD
 Sample : N4114-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E30

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M

Title : VOC Analysis

Signal : TIC: VV027261.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	74	82	93	rBV2	226460	260347	15.76%	1.978%
2	1.558	155	161	176	rVB	157620	182940	11.07%	1.390%
3	2.101	321	330	343	rVB	326564	458592	27.75%	3.485%
4	2.619	488	491	492	rBV2	934	503	0.03%	0.004%
5	2.899	576	578	581	rVB2	786	343	0.02%	0.003%
6	2.941	587	591	593	rBV2	766	595	0.04%	0.005%
7	2.989	604	606	609	rBV3	557	290	0.02%	0.002%
8	3.027	615	618	621	rBV2	794	585	0.04%	0.004%
9	3.124	646	648	650	rVB	697	284	0.02%	0.002%
10	3.159	653	659	662	rBV6	1187	1540	0.09%	0.012%
11	3.220	676	678	682	rVB2	787	408	0.02%	0.003%
12	3.285	697	698	701	rBV2	377	239	0.01%	0.002%
13	3.320	706	709	712	rBV3	494	466	0.03%	0.004%
14	3.359	715	721	726	rVB6	623	724	0.04%	0.006%
15	3.449	746	749	750	rBV	405	221	0.01%	0.002%
16	3.481	757	759	761	rVB2	688	287	0.02%	0.002%
17	3.539	774	777	783	rBV3	591	656	0.04%	0.005%
18	3.587	787	792	794	rBV3	585	440	0.03%	0.003%
19	3.648	809	811	813	rBV2	475	270	0.02%	0.002%
20	3.699	819	827	829	rBV2	489	599	0.04%	0.005%
21	3.760	844	846	849	rVB2	470	243	0.01%	0.002%
22	3.783	849	853	857	rVB2	780	680	0.04%	0.005%
23	3.805	857	860	862	rBV2	543	366	0.02%	0.003%
24	3.902	871	890	915	rBV3	261815	985495	59.64%	7.488%
25	4.342	1014	1027	1049	rBV2	263444	640664	38.77%	4.868%
26	4.632	1114	1117	1122	rBV6	830	812	0.05%	0.006%
27	4.664	1126	1127	1129	rBV2	588	225	0.01%	0.002%
28	4.796	1165	1168	1171	rBV3	657	375	0.02%	0.003%
29	4.825	1174	1177	1179	rBV3	589	398	0.02%	0.003%
30	4.905	1200	1202	1204	rBV3	413	216	0.01%	0.002%
31	5.040	1228	1244	1263	rBV2	645882	1652311	100.00%	12.555%
32	5.355	1340	1342	1343	rBV2	1162	452	0.03%	0.003%
33	5.439	1363	1368	1372	rBV6	1185	1432	0.09%	0.011%
34	5.612	1410	1422	1439	rBV	448254	907723	54.94%	6.897%
35	5.908	1505	1514	1531	rBV9	11770	28597	1.73%	0.217%
36	5.998	1540	1542	1545	rVB3	614	327	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081022\
 Data File : VV027261.D
 Acq On : 10 Aug 2022 16:41
 Operator : SY/MD
 Sample : N4114-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E30

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

37	6.066	1545	1563	1598	rBV	383733	823393	49.83%	6.256%
38	6.400	1665	1667	1670	rBV2	673	506	0.03%	0.004%
39	6.448	1680	1682	1685	rBV3	493	357	0.02%	0.003%
40	6.542	1710	1711	1714	rVB	526	195	0.01%	0.001%
41	6.561	1714	1717	1719	rBV	752	428	0.03%	0.003%
42	6.625	1735	1737	1739	rBV2	667	234	0.01%	0.002%
43	6.747	1773	1775	1778	rVB2	770	347	0.02%	0.003%
44	6.764	1778	1780	1784	rVB3	623	268	0.02%	0.002%
45	6.802	1789	1792	1794	rBV3	592	413	0.02%	0.003%
46	6.873	1811	1814	1817	rBV4	419	233	0.01%	0.002%
47	6.918	1826	1828	1831	rVB2	461	271	0.02%	0.002%
48	6.982	1833	1848	1881	rBV	187030	365193	22.10%	2.775%
49	7.243	1926	1929	1935	rVB5	1397	1401	0.08%	0.011%
50	7.268	1935	1937	1938	rBV5	518	220	0.01%	0.002%
51	7.313	1939	1951	1988	rVV	688143	1243279	75.24%	9.447%
52	7.619	2037	2046	2075	rBV2	130251	238486	14.43%	1.812%
53	7.895	2130	2132	2134	rBV2	505	254	0.02%	0.002%
54	7.931	2141	2143	2145	rBV2	395	205	0.01%	0.002%
55	7.966	2151	2154	2156	rBV	403	256	0.02%	0.002%
56	8.027	2171	2173	2177	rBV2	562	276	0.02%	0.002%
57	8.088	2181	2192	2233	rBV	538127	1023047	61.92%	7.773%
58	8.587	2344	2347	2349	rBV	629	445	0.03%	0.003%
59	8.638	2359	2363	2364	rBV2	710	403	0.02%	0.003%
60	8.725	2387	2390	2392	rVB3	859	507	0.03%	0.004%
61	8.850	2416	2429	2468	rBV	703192	1195380	72.35%	9.083%
62	9.075	2497	2499	2501	rBV2	969	599	0.04%	0.005%
63	9.117	2509	2512	2515	rBV4	686	433	0.03%	0.003%
64	9.136	2515	2518	2523	rVV	7988	4672	0.28%	0.035%
65	9.223	2541	2545	2550	rBV3	765	714	0.04%	0.005%
66	9.326	2576	2577	2581	rVB3	610	256	0.02%	0.002%
67	9.358	2581	2587	2591	rBV5	930	1034	0.06%	0.008%
68	9.394	2595	2598	2602	rBV3	439	314	0.02%	0.002%
69	9.471	2620	2622	2623	rBV2	457	228	0.01%	0.002%
70	9.564	2649	2651	2655	rVB3	666	301	0.02%	0.002%
71	9.599	2658	2662	2663	rBV2	570	353	0.02%	0.003%
72	9.625	2666	2670	2675	rBV5	954	895	0.05%	0.007%
73	9.792	2720	2722	2726	rVB	528	289	0.02%	0.002%
74	9.844	2736	2738	2739	rBV2	549	253	0.02%	0.002%
75	9.863	2741	2744	2746	rBV2	646	349	0.02%	0.003%
76	9.892	2751	2753	2754	rBV	446	212	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081022\
 Data File : VV027261.D
 Acq On : 10 Aug 2022 16:41
 Operator : SY/MD
 Sample : N4114-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E30

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

77	9.937	2765	2767	2770	rBV3	321	218	0.01%	0.002%
78	10.008	2787	2789	2791	rVB2	575	199	0.01%	0.002%
79	10.024	2792	2794	2797	rBV2	563	371	0.02%	0.003%
80	10.066	2804	2807	2808	rBV2	980	476	0.03%	0.004%
81	10.214	2841	2853	2872	rBV	586425	924963	55.98%	7.028%
82	10.384	2904	2906	2908	rBV	513	247	0.01%	0.002%
83	10.442	2920	2924	2927	rBV2	941	555	0.03%	0.004%
84	10.548	2955	2957	2959	rBV2	438	244	0.01%	0.002%
85	10.641	2984	2986	2989	rVB3	446	191	0.01%	0.001%
86	10.696	3001	3003	3006	rBV2	356	293	0.02%	0.002%
87	10.892	3063	3064	3067	rVB2	687	306	0.02%	0.002%
88	10.969	3085	3088	3090	rBV3	438	316	0.02%	0.002%
89	10.985	3090	3093	3095	rVV	566	325	0.02%	0.002%
90	11.143	3140	3142	3145	rBV3	486	326	0.02%	0.002%
91	11.249	3164	3175	3195	rBV	657258	1031034	62.40%	7.834%
92	11.548	3260	3268	3274	rBV8	3454	6193	0.37%	0.047%
93	11.622	3280	3291	3315	rBV	728551	1154170	69.85%	8.770%
94	12.075	3430	3432	3433	rBV	921	232	0.01%	0.002%
95	12.255	3486	3488	3490	rBV2	571	263	0.02%	0.002%
96	12.371	3521	3524	3526	rBV2	715	426	0.03%	0.003%
97	12.583	3587	3590	3594	rBV4	697	519	0.03%	0.004%
98	12.953	3703	3705	3709	rBV2	528	505	0.03%	0.004%
99	13.008	3720	3722	3723	rBV	679	325	0.02%	0.002%
100	13.133	3759	3761	3765	rVB3	837	540	0.03%	0.004%




Sum of corrected areas: 13160781

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081022\
Data File : VV027261.D
Acq On : 10 Aug 2022 16:41
Operator : SY/MD
Sample : N4114-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E30

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

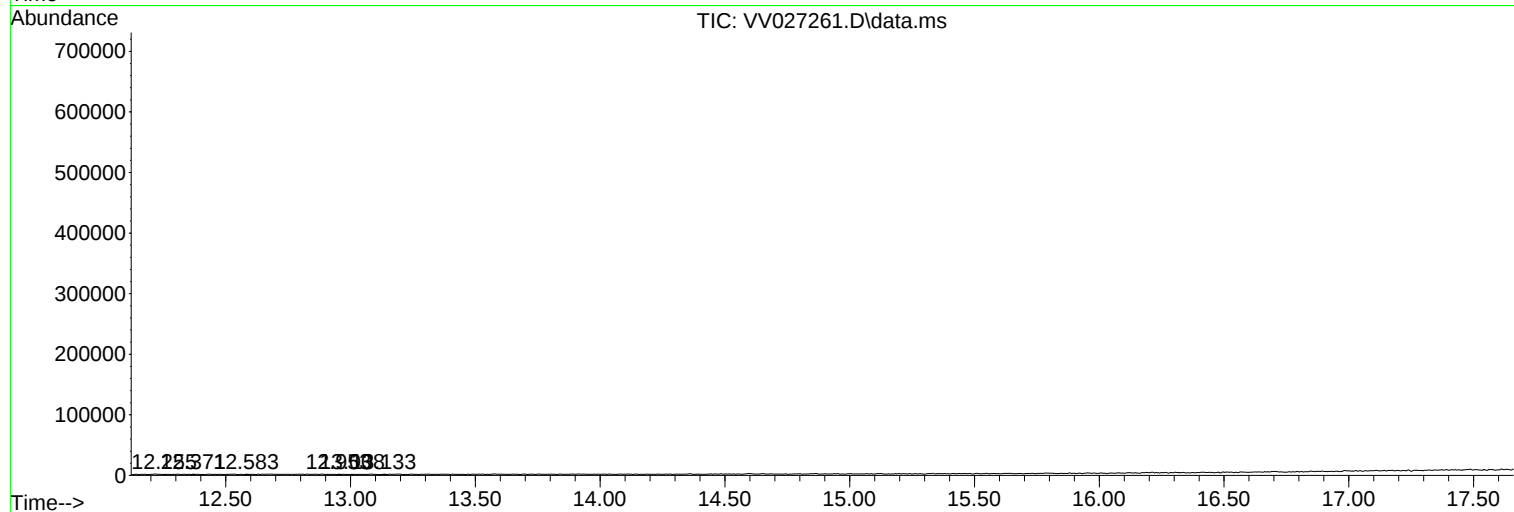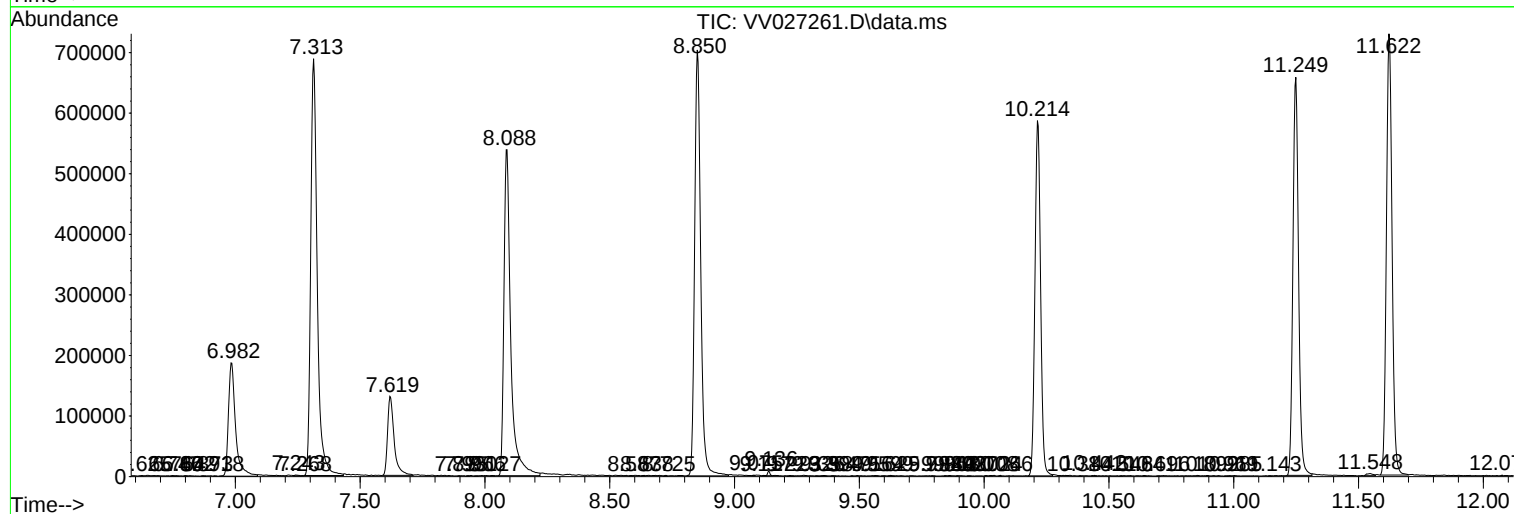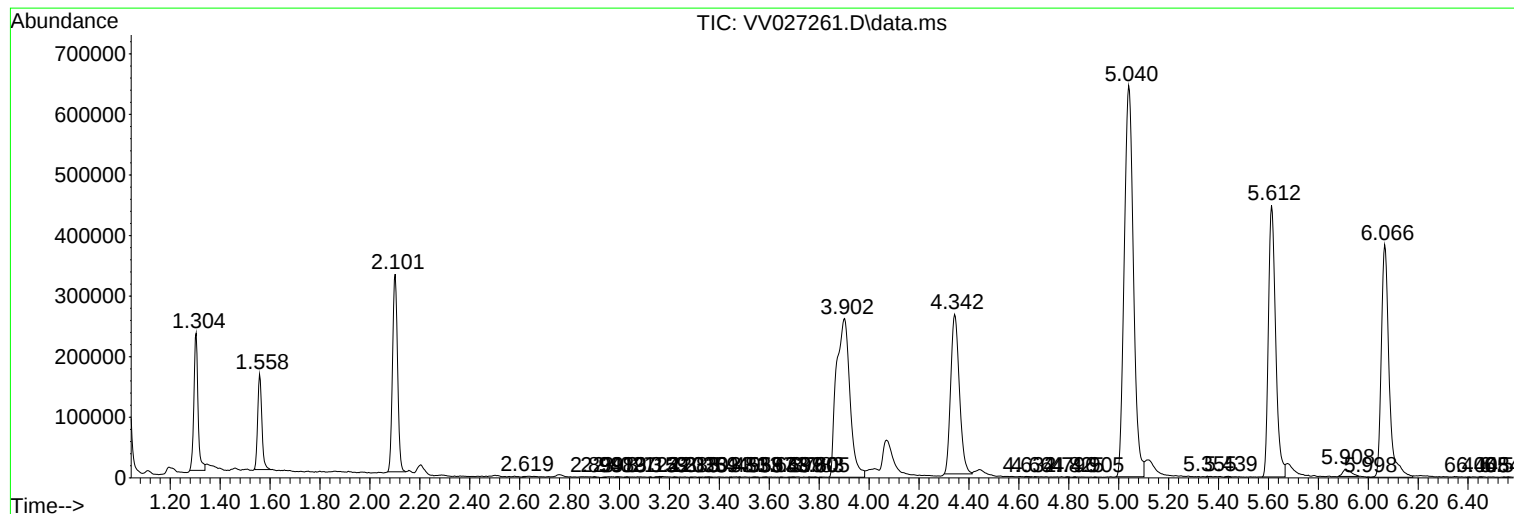

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081022\
Data File : VV027261.D
Acq On : 10 Aug 2022 16:41
Operator : SY/MD
Sample : N4114-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E30

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081022\
Data File : VV027261.D
Acq On : 10 Aug 2022 16:41
Operator : SY/MD
Sample : N4114-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E30

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc