

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081022\
 Data File : VV027264.D
 Acq On : 10 Aug 2022 17:56
 Operator : SY/MD
 Sample : N4114-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E33

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

Signal : TIC: VV027264.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	74	82	101	rBV2	221079	265919	16.66%	2.100%
2	1.558	155	161	180	rVB	154582	187865	11.77%	1.484%
3	2.102	321	330	343	rVB	318322	451662	28.30%	3.567%
4	2.487	447	450	452	rBV3	1622	1153	0.07%	0.009%
5	2.725	522	524	526	rBV3	546	360	0.02%	0.003%
6	2.757	528	534	544	rVV9	3412	5417	0.34%	0.043%
7	2.851	561	563	565	rBV2	846	401	0.03%	0.003%
8	2.999	605	609	614	rVB4	1013	554	0.03%	0.004%
9	3.018	614	615	617	rBV	537	240	0.02%	0.002%
10	3.034	617	620	621	rVB2	548	226	0.01%	0.002%
11	3.098	637	640	644	rBV2	504	380	0.02%	0.003%
12	3.217	674	677	680	rBV4	756	563	0.04%	0.004%
13	3.262	688	691	693	rBV3	505	313	0.02%	0.002%
14	3.307	702	705	707	rBV2	556	329	0.02%	0.003%
15	3.356	718	720	724	rVB2	480	266	0.02%	0.002%
16	3.381	726	728	733	rVV3	394	299	0.02%	0.002%
17	3.487	758	761	764	rVV2	581	338	0.02%	0.003%
18	3.500	764	765	769	rVB3	507	224	0.01%	0.002%
19	3.555	778	782	786	rBV3	410	331	0.02%	0.003%
20	3.613	798	800	802	rBV2	381	213	0.01%	0.002%
21	3.626	802	804	811	rVB3	640	681	0.04%	0.005%
22	3.658	811	814	816	rBV3	817	525	0.03%	0.004%
23	3.728	834	836	840	rVB3	791	561	0.04%	0.004%
24	3.764	844	847	853	rVB3	759	476	0.03%	0.004%
25	3.902	871	890	914	rBV2	261057	953882	59.77%	7.533%
26	4.343	1013	1027	1048	rBV	256182	633499	39.69%	5.003%
27	4.674	1128	1130	1132	rBV2	486	204	0.01%	0.002%
28	4.802	1168	1170	1172	rBV3	470	212	0.01%	0.002%
29	4.886	1194	1196	1200	rVB3	731	493	0.03%	0.004%
30	4.915	1200	1205	1206	rBV3	844	686	0.04%	0.005%
31	5.040	1227	1244	1263	rBV2	620733	1596031	100.00%	12.604%
32	5.613	1410	1422	1440	rBV	428836	872148	54.64%	6.887%
33	5.915	1504	1516	1534	rBV10	12646	32353	2.03%	0.255%
34	6.005	1540	1544	1545	rBV4	989	700	0.04%	0.006%
35	6.066	1549	1563	1601	rVV	369389	794869	49.80%	6.277%
36	6.381	1659	1661	1664	rBV4	815	388	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081022\
 Data File : VV027264.D
 Acq On : 10 Aug 2022 17:56
 Operator : SY/MD
 Sample : N4114-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E33

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

37	6.436	1676	1678	1679	rBV2	584	221	0.01%	0.002%
38	6.449	1679	1682	1684	rVV3	670	300	0.02%	0.002%
39	6.603	1726	1730	1733	rBV4	393	377	0.02%	0.003%
40	6.741	1771	1773	1775	rBV2	582	298	0.02%	0.002%
41	6.783	1781	1786	1788	rBV4	696	387	0.02%	0.003%
42	6.860	1806	1810	1813	rBV3	526	369	0.02%	0.003%
43	6.934	1830	1833	1836	rBV2	281	240	0.02%	0.002%
44	6.982	1838	1848	1875	rBV	175983	337510	21.15%	2.665%
45	7.269	1935	1937	1938	rBV	645	346	0.02%	0.003%
46	7.314	1940	1951	1987	rVV	651405	1178831	73.86%	9.309%
47	7.619	2037	2046	2076	rBV	123712	231134	14.48%	1.825%
48	7.944	2143	2147	2149	rBV3	624	492	0.03%	0.004%
49	7.986	2155	2160	2165	rBV5	1366	1121	0.07%	0.009%
50	8.014	2167	2169	2174	rVB4	712	357	0.02%	0.003%
51	8.037	2174	2176	2179	rVB3	533	286	0.02%	0.002%
52	8.088	2181	2192	2233	rBV	508090	984924	61.71%	7.778%
53	8.850	2418	2429	2451	rBV	682126	1123379	70.39%	8.871%
54	9.153	2521	2523	2525	rBV	519	216	0.01%	0.002%
55	9.188	2532	2534	2537	rVB2	810	416	0.03%	0.003%
56	9.265	2555	2558	2561	rBV2	606	415	0.03%	0.003%
57	9.330	2574	2578	2581	rBV2	534	290	0.02%	0.002%
58	9.352	2581	2585	2590	rBV4	1225	1175	0.07%	0.009%
59	9.452	2611	2616	2617	rVB2	581	328	0.02%	0.003%
60	9.468	2617	2621	2622	rBV2	370	230	0.01%	0.002%
61	9.481	2622	2625	2628	rVB2	505	333	0.02%	0.003%
62	9.526	2634	2639	2643	rBV4	700	682	0.04%	0.005%
63	9.545	2643	2645	2647	rBV2	446	219	0.01%	0.002%
64	9.796	2719	2723	2726	rBV2	598	524	0.03%	0.004%
65	9.834	2732	2735	2741	rVB4	882	747	0.05%	0.006%
66	9.915	2758	2760	2765	rBV3	644	499	0.03%	0.004%
67	9.937	2765	2767	2770	rBV2	466	250	0.02%	0.002%
68	9.953	2770	2772	2774	rBV2	445	226	0.01%	0.002%
69	9.982	2779	2781	2785	rVB3	760	444	0.03%	0.004%
70	10.027	2793	2795	2798	rVB3	768	379	0.02%	0.003%
71	10.053	2798	2803	2806	rBV	812	553	0.03%	0.004%
72	10.079	2808	2811	2812	rVB	468	237	0.01%	0.002%
73	10.214	2841	2853	2872	rBV	563033	901172	56.46%	7.116%
74	10.455	2926	2928	2931	rVB	674	264	0.02%	0.002%
75	10.484	2931	2937	2938	rBV4	682	495	0.03%	0.004%
76	10.571	2962	2964	2967	rVB3	600	259	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081022\
 Data File : VV027264.D
 Acq On : 10 Aug 2022 17:56
 Operator : SY/MD
 Sample : N4114-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E33

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

77	10.590	2967	2970	2975	rVB5	1040	798	0.05%	0.006%
78	10.632	2981	2983	2986	rVB3	546	330	0.02%	0.003%
79	10.735	3013	3015	3018	rVB2	565	242	0.02%	0.002%
80	10.966	3081	3087	3090	rVB4	627	599	0.04%	0.005%
81	10.982	3090	3092	3097	rBV2	615	604	0.04%	0.005%
82	11.014	3099	3102	3108	rVB4	729	552	0.03%	0.004%
83	11.149	3141	3144	3145	rBV2	495	304	0.02%	0.002%
84	11.204	3155	3161	3164	rBV4	691	814	0.05%	0.006%
85	11.249	3164	3175	3201	rBV	612266	974471	61.06%	7.695%
86	11.545	3260	3267	3274	rBV7	3738	6130	0.38%	0.048%
87	11.622	3279	3291	3314	rBV	695813	1097933	68.79%	8.670%
88	11.963	3395	3397	3399	rBV2	653	415	0.03%	0.003%
89	12.188	3464	3467	3468	rBV2	679	391	0.02%	0.003%
90	12.490	3558	3561	3563	rBV2	640	282	0.02%	0.002%
91	12.654	3610	3612	3615	rBV3	618	421	0.03%	0.003%
92	12.731	3634	3636	3640	rVB4	685	391	0.02%	0.003%
93	12.751	3640	3642	3645	rVB2	795	340	0.02%	0.003%
94	12.767	3645	3647	3648	rBV	549	270	0.02%	0.002%
95	13.043	3731	3733	3736	rBV3	582	308	0.02%	0.002%
96	13.191	3776	3779	3782	rBV2	681	501	0.03%	0.004%
97	13.207	3782	3784	3787	rVB	681	319	0.02%	0.003%
98	13.278	3804	3806	3809	rBV3	745	400	0.03%	0.003%
99	13.394	3839	3842	3843	rBV	496	239	0.01%	0.002%
100	13.882	3992	3994	3997	rBV3	746	578	0.04%	0.005%




Sum of corrected areas: 12663318

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081022\
Data File : VV027264.D
Acq On : 10 Aug 2022 17:56
Operator : SY/MD
Sample : N4114-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E33

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

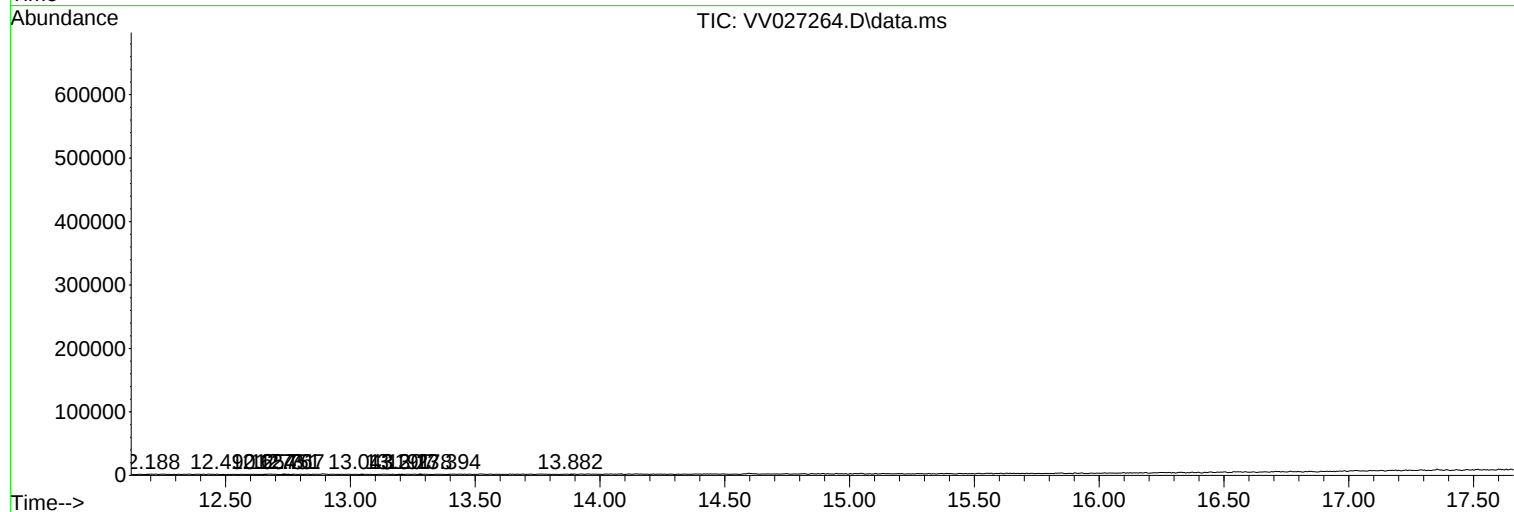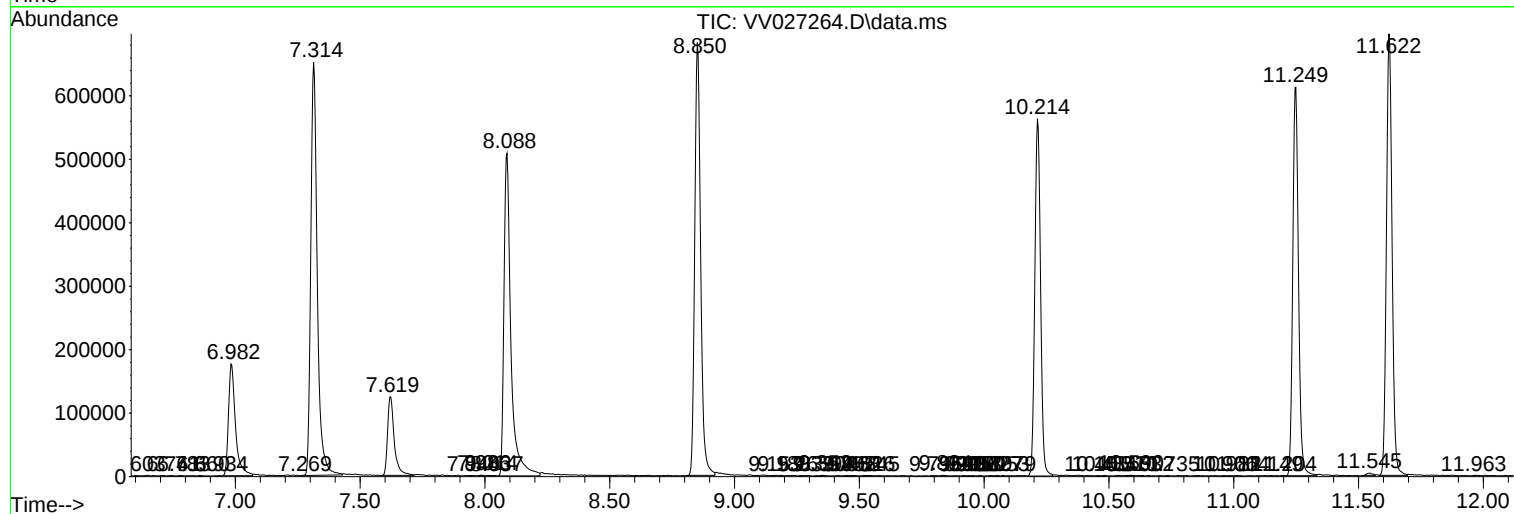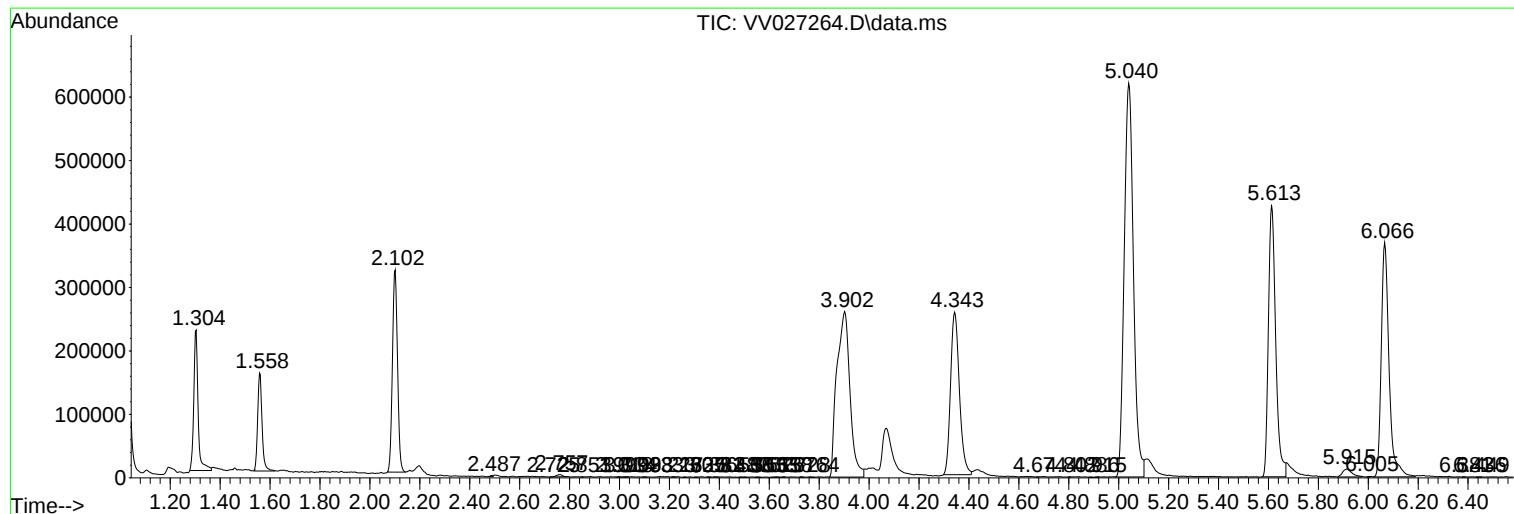

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081022\
Data File : VV027264.D
Acq On : 10 Aug 2022 17:56
Operator : SY/MD
Sample : N4114-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E33

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081022\
Data File : VV027264.D
Acq On : 10 Aug 2022 17:56
Operator : SY/MD
Sample : N4114-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E33

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc