

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081022\
 Data File : VV027268.D
 Acq On : 10 Aug 2022 19:35
 Operator : SY/MD
 Sample : N4114-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5D46

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

Signal : TIC: VV027268.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	109	rBV2	256951	291890	20.25%	2.420%
2	1.561	155	162	180	rVB	143733	177000	12.28%	1.468%
3	2.101	321	330	345	rBV	295451	417913	29.00%	3.465%
4	2.761	526	535	549	rBV6	16936	35382	2.46%	0.293%
5	2.854	561	564	565	rBV2	700	367	0.03%	0.003%
6	2.928	584	587	588	rBV2	701	343	0.02%	0.003%
7	2.995	605	608	610	rBV3	673	418	0.03%	0.003%
8	3.034	616	620	624	rBV5	671	701	0.05%	0.006%
9	3.114	642	645	646	rBV3	643	395	0.03%	0.003%
10	3.140	650	653	654	rBV2	700	423	0.03%	0.004%
11	3.195	668	670	674	rBV4	558	459	0.03%	0.004%
12	3.214	674	676	682	rBV2	792	670	0.05%	0.006%
13	3.375	723	726	727	rBV2	400	265	0.02%	0.002%
14	3.474	754	757	762	rVB5	626	509	0.04%	0.004%
15	3.497	762	764	767	rVB2	411	266	0.02%	0.002%
16	3.513	767	769	772	rBV2	543	312	0.02%	0.003%
17	3.561	778	784	786	rBV6	1058	907	0.06%	0.008%
18	3.671	814	818	819	rBV3	705	427	0.03%	0.004%
19	3.754	839	844	845	rBV2	415	330	0.02%	0.003%
20	3.780	849	852	854	rVB3	751	385	0.03%	0.003%
21	3.796	854	857	858	rBV	663	350	0.02%	0.003%
22	3.902	869	890	914	rBV3	446562	1382987	95.96%	11.467%
23	4.343	1012	1027	1051	rBV	225174	594100	41.22%	4.926%
24	4.767	1156	1159	1160	rBV2	387	260	0.02%	0.002%
25	5.040	1227	1244	1262	rBV2	560320	1441147	100.00%	11.950%
26	5.416	1357	1361	1364	rBV6	1141	873	0.06%	0.007%
27	5.545	1398	1401	1406	rVB4	1049	557	0.04%	0.005%
28	5.568	1406	1408	1410	rBV2	619	347	0.02%	0.003%
29	5.613	1410	1422	1439	rBV	397292	806146	55.94%	6.684%
30	5.969	1531	1533	1537	rBV4	648	459	0.03%	0.004%
31	6.011	1544	1546	1547	rBV	692	281	0.02%	0.002%
32	6.066	1550	1563	1603	rVV	335532	721472	50.06%	5.982%
33	6.394	1663	1665	1667	rVV3	777	286	0.02%	0.002%
34	6.416	1670	1672	1676	rBV3	516	360	0.02%	0.003%
35	6.455	1682	1684	1687	rBV4	665	303	0.02%	0.003%
36	6.468	1687	1688	1693	rVV4	610	380	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081022\
 Data File : VV027268.D
 Acq On : 10 Aug 2022 19:35
 Operator : SY/MD
 Sample : N4114-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5D46

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

37	6.519	1701	1704	1708	rBV3	822	635	0.04%	0.005%
38	6.577	1720	1722	1724	rBV2	563	336	0.02%	0.003%
39	6.632	1737	1739	1744	rVB3	560	356	0.02%	0.003%
40	6.786	1783	1787	1792	rVB6	524	459	0.03%	0.004%
41	6.809	1792	1794	1796	rBV2	577	371	0.03%	0.003%
42	6.825	1797	1799	1803	rVB2	1036	589	0.04%	0.005%
43	6.892	1819	1820	1823	rVB2	642	262	0.02%	0.002%
44	6.985	1838	1849	1873	rBV	154019	297365	20.63%	2.466%
45	7.259	1933	1934	1938	rVB3	813	481	0.03%	0.004%
46	7.313	1938	1951	1985	rBV	568237	1057398	73.37%	8.768%
47	7.619	2037	2046	2065	rBV	109461	200291	13.90%	1.661%
48	7.902	2132	2134	2138	rVB3	719	376	0.03%	0.003%
49	7.921	2138	2140	2144	rBV3	610	345	0.02%	0.003%
50	8.024	2170	2172	2175	rVB2	869	383	0.03%	0.003%
51	8.085	2181	2191	2225	rBV	437417	853123	59.20%	7.074%
52	8.693	2377	2380	2382	rBV3	687	476	0.03%	0.004%
53	8.751	2393	2398	2402	rVV4	718	792	0.05%	0.007%
54	8.850	2418	2429	2455	rBV	629415	1056284	73.29%	8.758%
55	9.040	2486	2488	2490	rBV3	946	512	0.04%	0.004%
56	9.333	2575	2579	2581	rBV3	688	539	0.04%	0.004%
57	9.346	2581	2583	2586	rVB	801	336	0.02%	0.003%
58	9.358	2586	2587	2589	rBV2	569	312	0.02%	0.003%
59	9.416	2601	2605	2607	rBV3	618	439	0.03%	0.004%
60	9.442	2610	2613	2615	rBV2	706	418	0.03%	0.003%
61	9.464	2615	2620	2621	rBV2	440	365	0.03%	0.003%
62	9.474	2621	2623	2626	rVB2	586	277	0.02%	0.002%
63	9.538	2641	2643	2650	rBV5	580	688	0.05%	0.006%
64	9.616	2665	2667	2669	rBV4	676	333	0.02%	0.003%
65	9.715	2696	2698	2702	rVB3	489	300	0.02%	0.002%
66	9.792	2720	2722	2727	rVB3	746	530	0.04%	0.004%
67	9.818	2728	2730	2733	rVB2	435	278	0.02%	0.002%
68	9.850	2737	2740	2746	rBV3	620	672	0.05%	0.006%
69	9.953	2770	2772	2773	rBV2	843	248	0.02%	0.002%
70	10.046	2797	2801	2805	rVB3	795	664	0.05%	0.006%
71	10.120	2820	2824	2825	rBV3	727	502	0.03%	0.004%
72	10.172	2837	2840	2841	rBV2	1003	448	0.03%	0.004%
73	10.214	2841	2853	2875	rVV	521593	812562	56.38%	6.738%
74	10.400	2909	2911	2915	rBV3	598	376	0.03%	0.003%
75	10.628	2979	2982	2984	rBV3	736	447	0.03%	0.004%
76	10.728	3011	3013	3015	rBV2	436	257	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081022\
 Data File : VV027268.D
 Acq On : 10 Aug 2022 19:35
 Operator : SY/MD
 Sample : N4114-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5D46

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

77	10.841	3044	3048	3049	rBV3	490	261	0.02%	0.002%
78	10.905	3063	3068	3071	rBV2	528	461	0.03%	0.004%
79	10.960	3082	3085	3086	rBV	531	268	0.02%	0.002%
80	11.098	3124	3128	3131	rBV4	841	613	0.04%	0.005%
81	11.249	3160	3175	3195	rBV	572842	901051	62.52%	7.471%
82	11.622	3280	3291	3313	rBV	626188	978085	67.87%	8.110%
83	11.828	3353	3355	3357	rBV2	625	302	0.02%	0.003%
84	11.844	3357	3360	3361	rBV2	578	250	0.02%	0.002%
85	11.908	3378	3380	3386	rVB3	1072	667	0.05%	0.006%
86	11.934	3386	3388	3390	rBV2	690	328	0.02%	0.003%
87	11.950	3390	3393	3396	rVB2	798	473	0.03%	0.004%
88	11.969	3396	3399	3405	rBV5	722	718	0.05%	0.006%
89	12.159	3455	3458	3461	rBV3	971	647	0.04%	0.005%
90	12.236	3480	3482	3483	rBV3	730	292	0.02%	0.002%
91	12.451	3546	3549	3551	rBV4	498	342	0.02%	0.003%
92	12.760	3643	3645	3650	rBV2	666	312	0.02%	0.003%
93	12.979	3710	3713	3716	rBV3	530	368	0.03%	0.003%
94	13.075	3740	3743	3745	rBV3	742	495	0.03%	0.004%
95	13.156	3766	3768	3770	rBV	894	404	0.03%	0.003%
96	13.271	3801	3804	3806	rBV2	818	538	0.04%	0.004%
97	13.390	3838	3841	3843	rBV3	852	506	0.04%	0.004%
98	13.516	3878	3880	3882	rBV2	750	384	0.03%	0.003%
99	14.133	4069	4072	4074	rBV3	807	463	0.03%	0.004%
100	14.300	4121	4124	4125	rBV2	853	513	0.04%	0.004%




Sum of corrected areas: 12060236

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081022\
Data File : VV027268.D
Acq On : 10 Aug 2022 19:35
Operator : SY/MD
Sample : N4114-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5D46

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

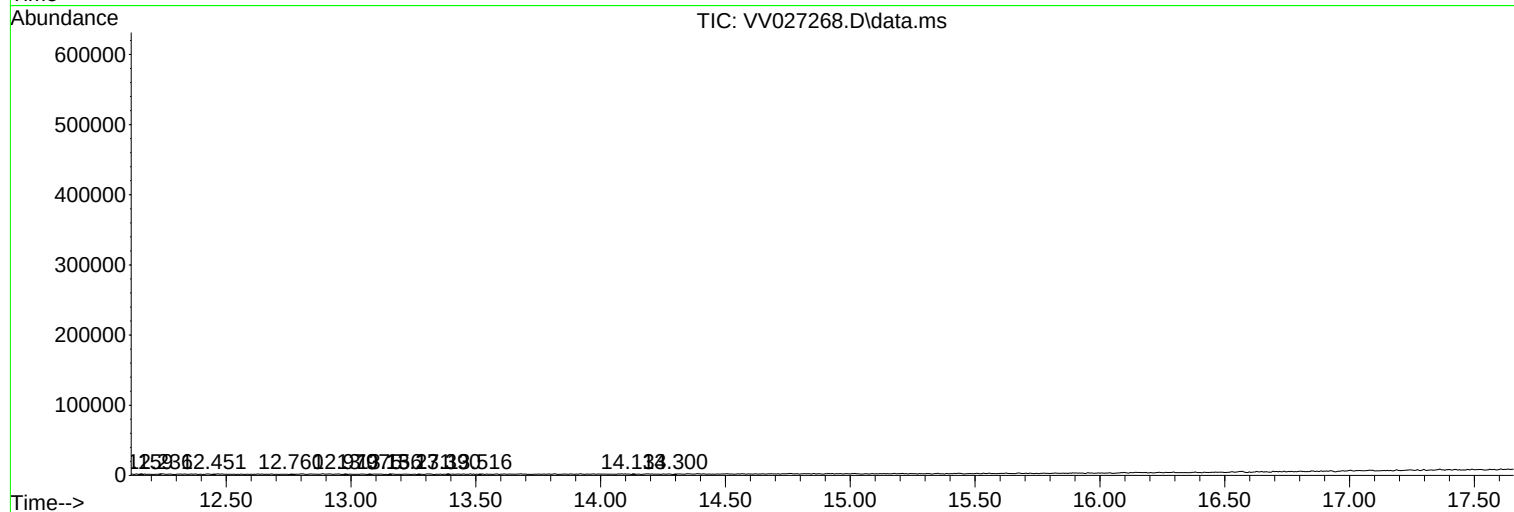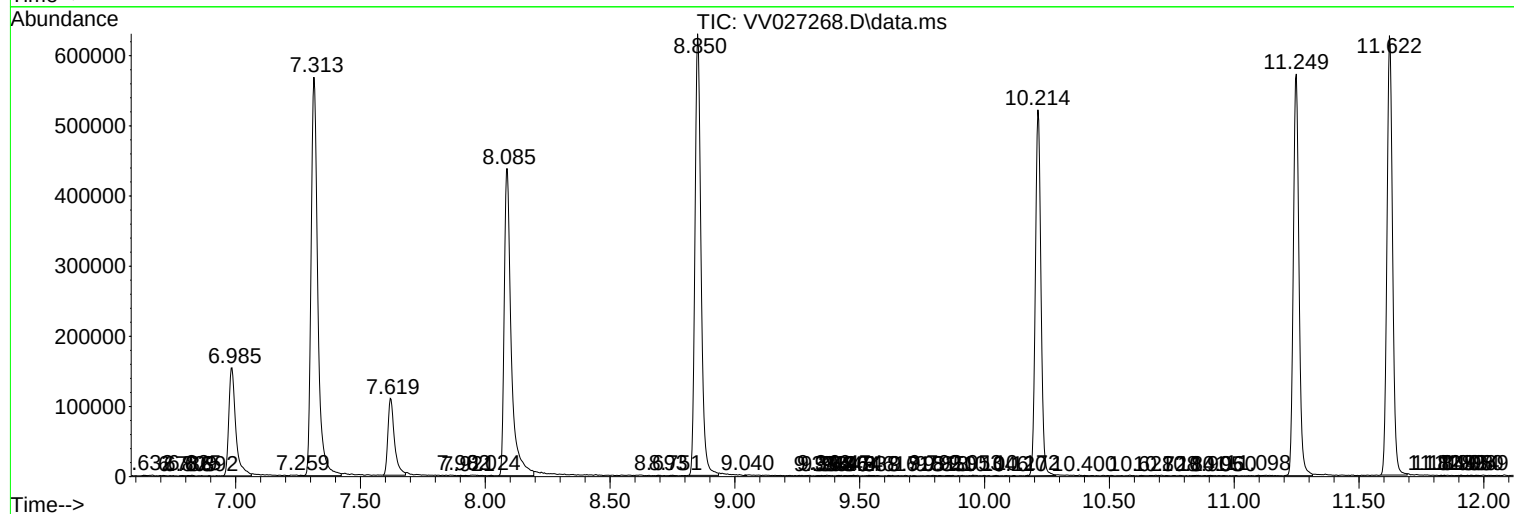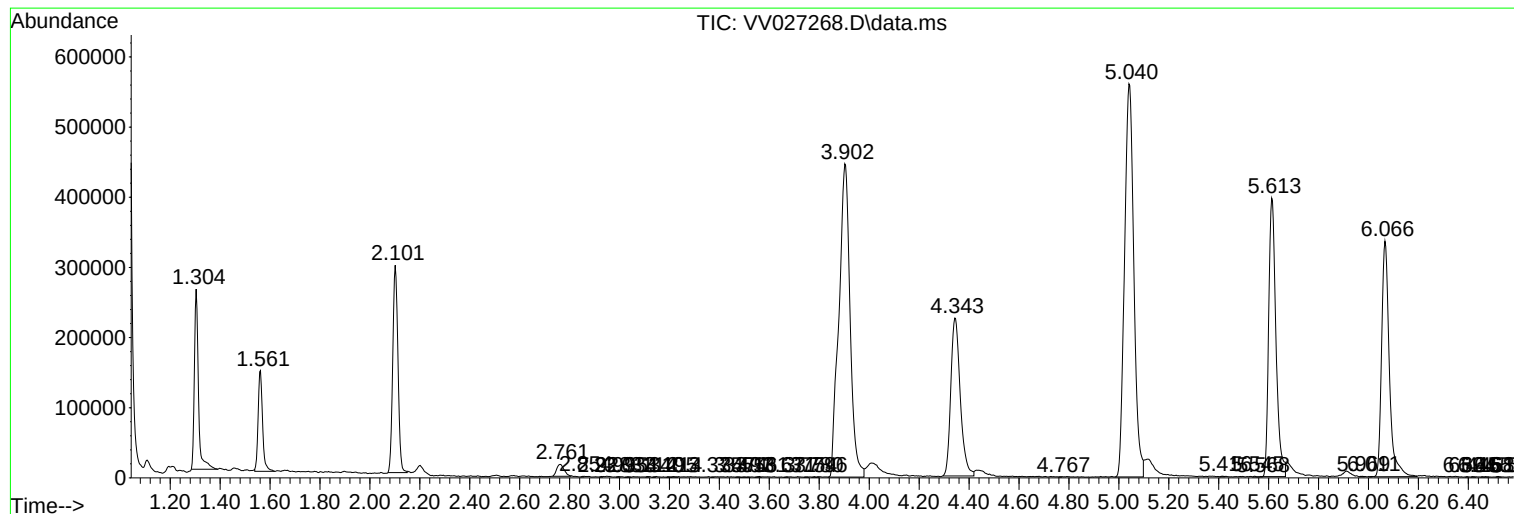

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081022\
Data File : VV027268.D
Acq On : 10 Aug 2022 19:35
Operator : SY/MD
Sample : N4114-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5D46

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081022\
Data File : VV027268.D
Acq On : 10 Aug 2022 19:35
Operator : SY/MD
Sample : N4114-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5D46

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc