

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081022\
 Data File : VV027269.D
 Acq On : 10 Aug 2022 20:00
 Operator : SY/MD
 Sample : N4144-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY144

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

Signal : TIC: VV027269.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	88	rBV	159299	159439	11.13%	1.479%
2	1.558	156	161	174	rVB	142469	167828	11.72%	1.557%
3	2.101	322	330	343	rVB	292139	407517	28.45%	3.780%
4	2.966	596	599	602	rBV2	722	482	0.03%	0.004%
5	3.002	608	610	613	rBV4	833	548	0.04%	0.005%
6	3.053	623	626	629	rBV3	674	592	0.04%	0.005%
7	3.384	727	729	731	rBV2	522	306	0.02%	0.003%
8	3.522	769	772	774	rBV2	788	316	0.02%	0.003%
9	3.667	812	817	819	rBV3	479	372	0.03%	0.003%
10	3.699	823	827	832	rVB2	528	491	0.03%	0.005%
11	3.738	835	839	840	rBV2	512	293	0.02%	0.003%
12	3.789	854	855	861	rVB3	672	381	0.03%	0.004%
13	3.821	861	865	868	rVB4	358	293	0.02%	0.003%
14	3.870	868	880	910	rBV	144456	388296	27.11%	3.601%
15	4.342	1012	1027	1049	rBV	234829	592887	41.39%	5.499%
16	4.696	1134	1137	1138	rBV3	588	365	0.03%	0.003%
17	4.760	1154	1157	1158	rBV2	682	369	0.03%	0.003%
18	4.847	1182	1184	1187	rBV3	737	367	0.03%	0.003%
19	4.918	1202	1206	1207	rBV3	578	362	0.03%	0.003%
20	4.976	1222	1224	1226	rBV	507	283	0.02%	0.003%
21	5.040	1228	1244	1263	rBV2	557243	1432438	100.00%	13.286%
22	5.429	1363	1365	1367	rBV2	557	296	0.02%	0.003%
23	5.503	1385	1388	1392	rBV4	677	657	0.05%	0.006%
24	5.535	1396	1398	1401	rBV2	944	509	0.04%	0.005%
25	5.612	1411	1422	1466	rBV	381370	811114	56.62%	7.523%
26	5.828	1487	1489	1493	rBV3	1187	871	0.06%	0.008%
27	5.911	1506	1515	1528	rBV3	3568	7693	0.54%	0.071%
28	5.989	1533	1539	1541	rBV4	968	970	0.07%	0.009%
29	6.066	1548	1563	1593	rBV	336517	720349	50.29%	6.681%
30	6.313	1638	1640	1644	rBV3	642	363	0.03%	0.003%
31	6.349	1648	1651	1655	rBV5	610	436	0.03%	0.004%
32	6.516	1701	1703	1706	rBV4	453	267	0.02%	0.002%
33	6.593	1726	1727	1731	rBV2	444	333	0.02%	0.003%
34	6.657	1743	1747	1749	rBV3	1341	966	0.07%	0.009%
35	6.773	1780	1783	1787	rBV4	436	359	0.03%	0.003%
36	6.915	1824	1827	1829	rVB2	659	302	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081022\
 Data File : VV027269.D
 Acq On : 10 Aug 2022 20:00
 Operator : SY/MD
 Sample : N4144-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY144

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

37	6.927	1829	1831	1836	rBV4	539	390	0.03%	0.004%
38	6.985	1838	1849	1878	rBV	151430	293773	20.51%	2.725%
39	7.207	1913	1918	1919	rBV3	840	668	0.05%	0.006%
40	7.313	1937	1951	1985	rBV	569926	1041740	72.72%	9.662%
41	7.619	2037	2046	2066	rBV	109954	196647	13.73%	1.824%
42	7.937	2143	2145	2148	rBV4	654	515	0.04%	0.005%
43	8.024	2169	2172	2175	rBV4	1108	720	0.05%	0.007%
44	8.088	2181	2192	2221	rBV	462518	866130	60.47%	8.033%
45	8.522	2325	2327	2331	rVB3	866	505	0.04%	0.005%
46	8.609	2351	2354	2355	rBV3	588	332	0.02%	0.003%
47	8.657	2367	2369	2373	rBV5	542	287	0.02%	0.003%
48	8.677	2373	2375	2380	rVB4	544	318	0.02%	0.003%
49	8.850	2418	2429	2451	rBV	593863	1010416	70.54%	9.372%
50	9.226	2543	2546	2547	rBV3	725	385	0.03%	0.004%
51	9.265	2556	2558	2559	rBV2	671	273	0.02%	0.003%
52	9.297	2563	2568	2569	rBV2	802	618	0.04%	0.006%
53	9.371	2588	2591	2592	rBV	756	419	0.03%	0.004%
54	9.432	2607	2610	2615	rBV4	958	646	0.05%	0.006%
55	9.564	2645	2651	2654	rBV3	893	1000	0.07%	0.009%
56	9.664	2679	2682	2685	rBV4	656	345	0.02%	0.003%
57	9.693	2689	2691	2694	rVB3	873	376	0.03%	0.003%
58	9.738	2700	2705	2707	rBV4	869	669	0.05%	0.006%
59	9.812	2726	2728	2730	rBV2	630	287	0.02%	0.003%
60	10.014	2789	2791	2793	rBV3	623	366	0.03%	0.003%
61	10.104	2812	2819	2821	rBV4	539	518	0.04%	0.005%
62	10.136	2827	2829	2832	rVB3	822	320	0.02%	0.003%
63	10.172	2838	2840	2841	rBV2	533	259	0.02%	0.002%
64	10.214	2842	2853	2875	rVV	517061	826210	57.68%	7.663%
65	10.313	2881	2884	2887	rBV3	883	482	0.03%	0.004%
66	10.416	2912	2916	2919	rBV5	884	633	0.04%	0.006%
67	10.471	2930	2933	2939	rBV3	777	526	0.04%	0.005%
68	10.648	2985	2988	2991	rBV3	661	506	0.04%	0.005%
69	10.670	2991	2995	2997	rVB2	464	368	0.03%	0.003%
70	10.834	3043	3046	3048	rBV2	592	372	0.03%	0.003%
71	10.992	3091	3095	3096	rBV2	665	370	0.03%	0.003%
72	11.027	3104	3106	3112	rVB2	754	454	0.03%	0.004%
73	11.053	3112	3114	3116	rBV	611	265	0.02%	0.002%
74	11.191	3151	3157	3161	rBV5	820	1053	0.07%	0.010%
75	11.249	3161	3175	3194	rBV	537238	845875	59.05%	7.846%
76	11.545	3258	3267	3280	rBV5	5833	13120	0.92%	0.122%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081022\
 Data File : VV027269.D
 Acq On : 10 Aug 2022 20:00
 Operator : SY/MD
 Sample : N4144-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY144

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

77	11.622	3280	3291	3311	rVV	602069	959544	66.99%	8.900%
78	11.824	3352	3354	3357	rVB3	1250	508	0.04%	0.005%
79	11.847	3357	3361	3363	rBV5	1061	787	0.05%	0.007%
80	11.947	3388	3392	3395	rBV3	720	644	0.04%	0.006%
81	12.059	3423	3427	3429	rBV3	827	518	0.04%	0.005%
82	12.072	3429	3431	3434	rBV3	729	434	0.03%	0.004%
83	12.091	3434	3437	3439	rBV2	726	469	0.03%	0.004%
84	12.181	3463	3465	3468	rVB	1207	472	0.03%	0.004%
85	12.204	3468	3472	3474	rBV3	730	598	0.04%	0.006%
86	12.493	3558	3562	3564	rBV2	748	592	0.04%	0.005%
87	12.535	3572	3575	3579	rVB4	623	418	0.03%	0.004%
88	12.828	3663	3666	3669	rBV	510	432	0.03%	0.004%
89	12.856	3672	3675	3681	rVV4	812	665	0.05%	0.006%
90	13.082	3743	3745	3749	rVB4	750	486	0.03%	0.005%
91	13.130	3757	3760	3764	rBV3	704	406	0.03%	0.004%
92	13.262	3798	3801	3807	rBV5	1047	910	0.06%	0.008%
93	13.323	3817	3820	3824	rVB4	1052	826	0.06%	0.008%
94	13.358	3828	3831	3835	rVB3	774	596	0.04%	0.006%
95	13.429	3852	3853	3855	rBV3	612	291	0.02%	0.003%
96	13.943	4009	4013	4018	rBV5	775	870	0.06%	0.008%
97	14.204	4090	4094	4095	rBV	630	422	0.03%	0.004%
98	14.262	4110	4112	4114	rBV2	850	331	0.02%	0.003%
99	14.336	4133	4135	4138	rBV4	1042	690	0.05%	0.006%
100	14.795	4273	4278	4279	rBV3	993	786	0.05%	0.007%




Sum of corrected areas: 10781561

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081022\
Data File : VV027269.D
Acq On : 10 Aug 2022 20:00
Operator : SY/MD
Sample : N4144-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY144

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

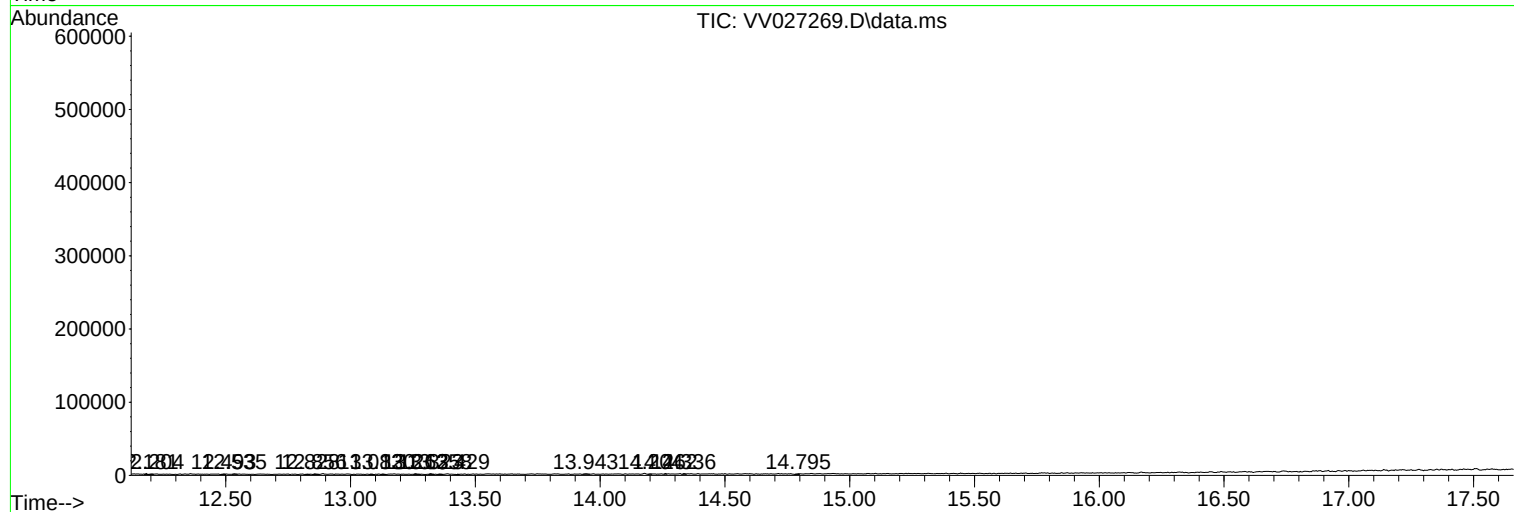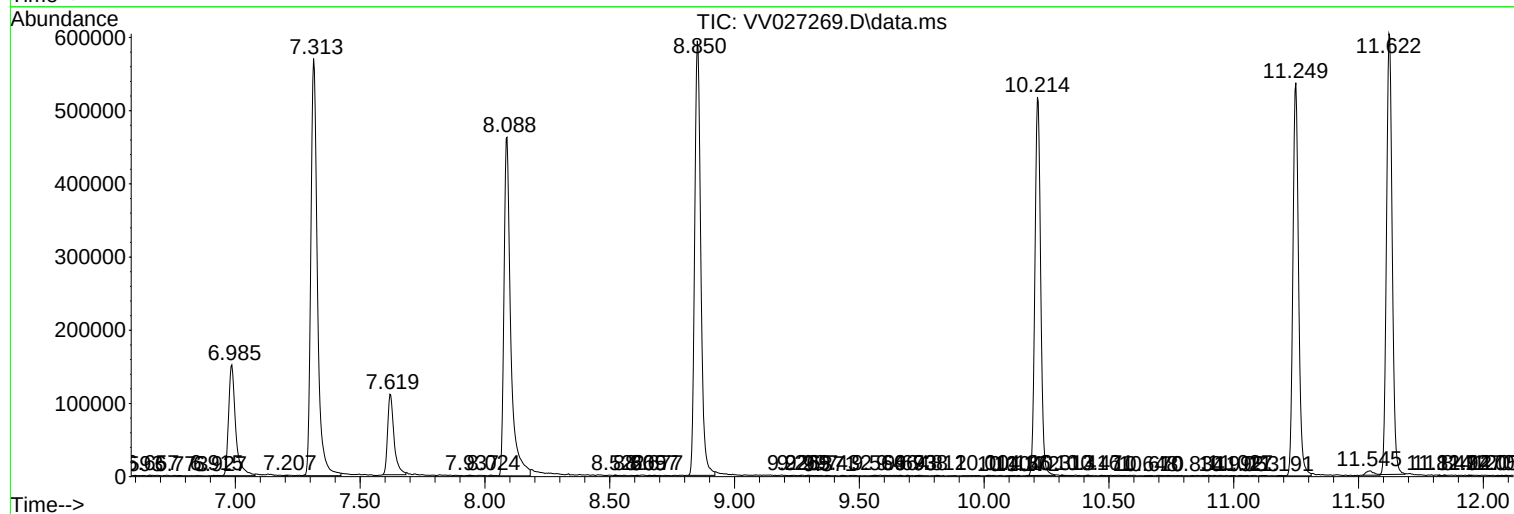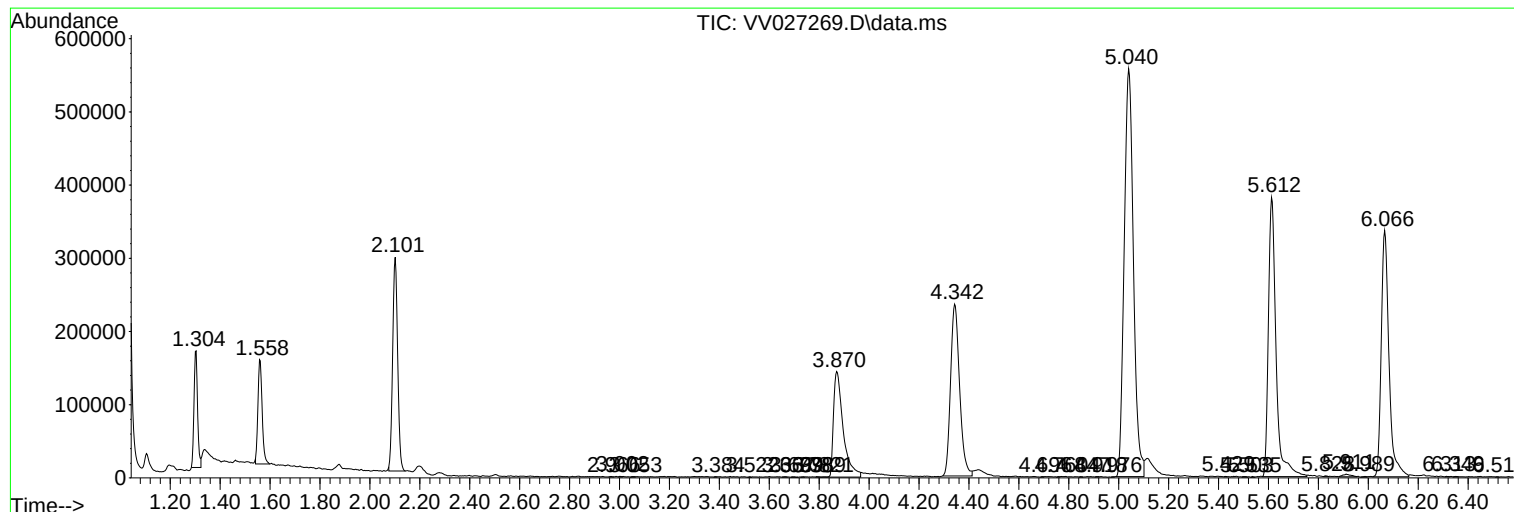

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081022\
Data File : VV027269.D
Acq On : 10 Aug 2022 20:00
Operator : SY/MD
Sample : N4144-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY144

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081022\
Data File : VV027269.D
Acq On : 10 Aug 2022 20:00
Operator : SY/MD
Sample : N4144-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY144

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc