

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081022\
 Data File : VV027270.D
 Acq On : 10 Aug 2022 20:25
 Operator : SY/MD
 Sample : N4144-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY147

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

Signal : TIC: VV027270.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	88	rBV	168395	171497	11.72%	1.541%
2	1.561	156	162	176	rVB	151886	182573	12.48%	1.641%
3	2.101	321	330	341	rVB	297220	414208	28.31%	3.723%
4	2.863	565	567	569	rBV3	608	361	0.02%	0.003%
5	2.940	589	591	595	rBV4	818	451	0.03%	0.004%
6	3.104	638	642	647	rVB3	1107	872	0.06%	0.008%
7	3.130	647	650	651	rBV	552	291	0.02%	0.003%
8	3.185	651	667	683	rBV2	26386	57654	3.94%	0.518%
9	3.375	724	726	728	rBV2	550	193	0.01%	0.002%
10	3.455	749	751	753	rBV3	443	257	0.02%	0.002%
11	3.484	758	760	761	rBV	478	169	0.01%	0.002%
12	3.497	761	764	766	rBV2	521	302	0.02%	0.003%
13	3.590	787	793	795	rBV3	598	484	0.03%	0.004%
14	3.661	813	815	816	rBV3	500	170	0.01%	0.002%
15	3.728	832	836	839	rBV4	717	475	0.03%	0.004%
16	3.744	839	841	844	rVB3	644	281	0.02%	0.003%
17	3.773	844	850	856	rVB6	697	851	0.06%	0.008%
18	3.802	857	859	861	rBV2	446	249	0.02%	0.002%
19	3.828	863	867	870	rBV3	835	667	0.05%	0.006%
20	3.870	870	880	917	rBV	150112	458247	31.32%	4.119%
21	4.342	1012	1027	1048	rBV	245544	606195	41.43%	5.449%
22	4.551	1090	1092	1093	rBV2	853	347	0.02%	0.003%
23	4.738	1147	1150	1152	rBV2	673	452	0.03%	0.004%
24	4.796	1165	1168	1172	rBV4	884	623	0.04%	0.006%
25	4.825	1175	1177	1178	rBV2	458	174	0.01%	0.002%
26	4.866	1188	1190	1194	rVB2	868	535	0.04%	0.005%
27	4.895	1194	1199	1203	rBV6	1029	965	0.07%	0.009%
28	4.924	1203	1208	1211	rBV4	512	581	0.04%	0.005%
29	5.040	1228	1244	1262	rBV2	570252	1463280	100.00%	13.152%
30	5.455	1370	1373	1374	rBV3	1073	651	0.04%	0.006%
31	5.545	1399	1401	1402	rBV3	417	184	0.01%	0.002%
32	5.612	1410	1422	1439	rBV	389540	793570	54.23%	7.133%
33	5.969	1531	1533	1534	rBV2	816	338	0.02%	0.003%
34	6.066	1550	1563	1592	rBV	339579	723717	49.46%	6.505%
35	6.429	1674	1676	1680	rBV5	661	485	0.03%	0.004%
36	6.497	1695	1697	1699	rVB2	876	344	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081022\
 Data File : VV027270.D
 Acq On : 10 Aug 2022 20:25
 Operator : SY/MD
 Sample : N4144-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY147

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

37	6.513	1699	1702	1706	rVB3	1169	735	0.05%	0.007%
38	6.538	1707	1710	1715	rBV3	615	522	0.04%	0.005%
39	6.603	1728	1730	1733	rVB3	831	456	0.03%	0.004%
40	6.628	1734	1738	1741	rBV5	494	440	0.03%	0.004%
41	6.657	1741	1747	1750	rBV6	1028	1203	0.08%	0.011%
42	6.731	1768	1770	1771	rBV2	643	215	0.01%	0.002%
43	6.789	1785	1788	1792	rVB2	973	687	0.05%	0.006%
44	6.815	1792	1796	1797	rBV3	771	551	0.04%	0.005%
45	6.982	1838	1848	1877	rBV	153172	297504	20.33%	2.674%
46	7.313	1939	1951	1973	rBV	592015	1057656	72.28%	9.507%
47	7.619	2036	2046	2071	rBV2	113525	206234	14.09%	1.854%
48	7.931	2140	2143	2144	rBV2	1337	858	0.06%	0.008%
49	8.088	2180	2192	2227	rBV	466275	887119	60.63%	7.974%
50	8.596	2348	2350	2354	rBV3	814	739	0.05%	0.007%
51	8.751	2396	2398	2400	rBV2	568	274	0.02%	0.002%
52	8.802	2411	2414	2416	rBV2	671	474	0.03%	0.004%
53	8.850	2418	2429	2453	rVV	632976	1042639	71.25%	9.372%
54	9.069	2490	2497	2498	rBV5	1245	1184	0.08%	0.011%
55	9.178	2529	2531	2533	rBV4	557	291	0.02%	0.003%
56	9.230	2544	2547	2550	rVB2	930	598	0.04%	0.005%
57	9.300	2567	2569	2573	rVB2	1072	583	0.04%	0.005%
58	9.320	2573	2575	2577	rBV3	798	420	0.03%	0.004%
59	9.384	2593	2595	2596	rBV	626	254	0.02%	0.002%
60	9.410	2600	2603	2607	rBV2	668	433	0.03%	0.004%
61	9.429	2607	2609	2611	rBV2	838	272	0.02%	0.002%
62	9.599	2659	2662	2664	rBV2	562	306	0.02%	0.003%
63	9.667	2681	2683	2686	rBV4	681	367	0.03%	0.003%
64	9.686	2686	2689	2691	rVV3	475	272	0.02%	0.002%
65	9.725	2697	2701	2702	rBV4	742	545	0.04%	0.005%
66	9.805	2724	2726	2728	rVB2	710	315	0.02%	0.003%
67	9.821	2729	2731	2735	rBV3	746	410	0.03%	0.004%
68	9.876	2744	2748	2750	rBV2	532	442	0.03%	0.004%
69	9.898	2753	2755	2757	rVB3	638	244	0.02%	0.002%
70	9.911	2757	2759	2763	rBV4	778	585	0.04%	0.005%
71	9.947	2767	2770	2771	rBV3	775	411	0.03%	0.004%
72	10.021	2786	2793	2795	rBV3	1388	1484	0.10%	0.013%
73	10.213	2841	2853	2872	rBV	523537	835392	57.09%	7.509%
74	10.397	2904	2910	2914	rBV4	792	841	0.06%	0.008%
75	10.464	2927	2931	2934	rVB3	726	532	0.04%	0.005%
76	10.487	2934	2938	2940	rBV2	892	507	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081022\
 Data File : VV027270.D
 Acq On : 10 Aug 2022 20:25
 Operator : SY/MD
 Sample : N4144-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY147

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

77	10.513	2940	2946	2951	rBV6	1125	1449	0.10%	0.013%
78	10.577	2961	2966	2970	rVB5	974	986	0.07%	0.009%
79	10.603	2970	2974	2976	rBV4	1400	963	0.07%	0.009%
80	10.673	2994	2996	2997	rBV	485	185	0.01%	0.002%
81	10.722	3007	3011	3015	rBV4	471	592	0.04%	0.005%
82	10.818	3039	3041	3044	rVB3	486	236	0.02%	0.002%
83	10.853	3044	3052	3055	rBV5	1768	2169	0.15%	0.019%
84	10.898	3064	3066	3068	rVB2	497	169	0.01%	0.002%
85	10.924	3071	3074	3077	rBV3	674	555	0.04%	0.005%
86	11.075	3120	3121	3125	rVB4	673	320	0.02%	0.003%
87	11.107	3130	3131	3134	rBV2	551	349	0.02%	0.003%
88	11.249	3161	3175	3200	rBV	562798	892018	60.96%	8.018%
89	11.419	3225	3228	3229	rBV3	743	441	0.03%	0.004%
90	11.622	3281	3291	3308	rBV	636212	991915	67.79%	8.916%
91	11.914	3379	3382	3385	rVB4	674	476	0.03%	0.004%
92	11.934	3386	3388	3393	rBV4	722	639	0.04%	0.006%
93	12.310	3501	3505	3509	rBV6	865	808	0.06%	0.007%
94	12.680	3618	3620	3623	rVB3	818	403	0.03%	0.004%
95	12.844	3669	3671	3675	rBV2	533	369	0.03%	0.003%
96	12.969	3707	3710	3713	rVB2	518	385	0.03%	0.003%
97	13.127	3756	3759	3762	rBV2	619	508	0.03%	0.005%
98	13.416	3847	3849	3852	rBV2	785	475	0.03%	0.004%
99	13.686	3931	3933	3935	rBV2	529	305	0.02%	0.003%
100	13.863	3984	3988	3994	rBV4	858	1174	0.08%	0.011%




Sum of corrected areas: 11125576

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081022\
Data File : VV027270.D
Acq On : 10 Aug 2022 20:25
Operator : SY/MD
Sample : N4144-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY147

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

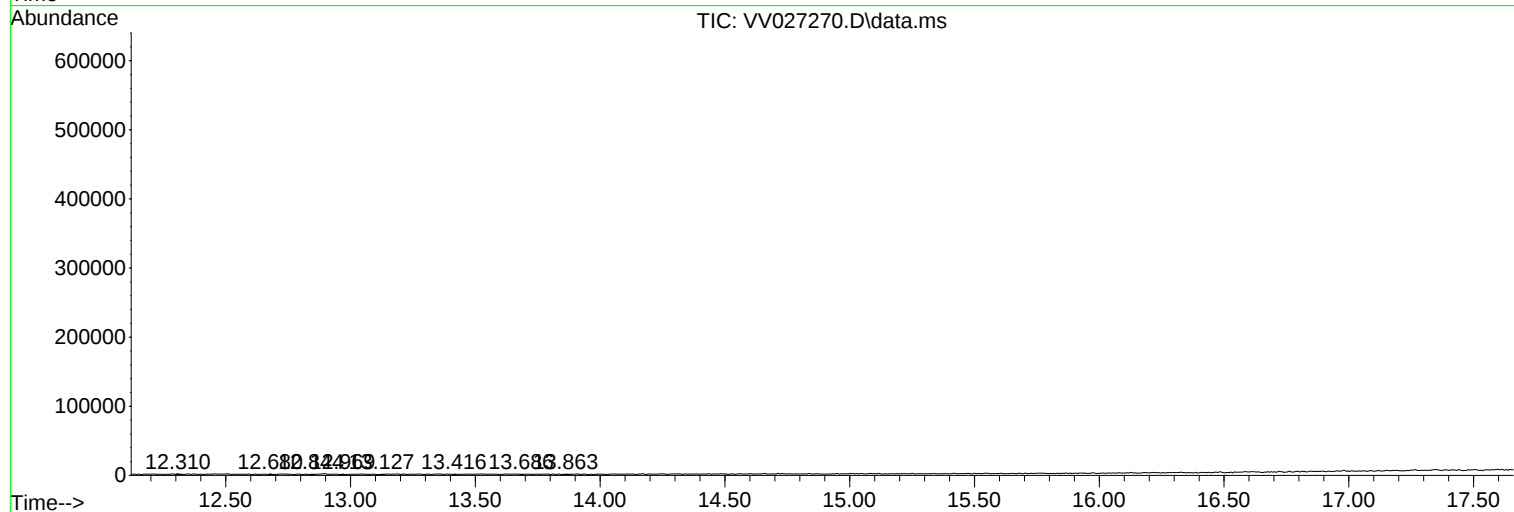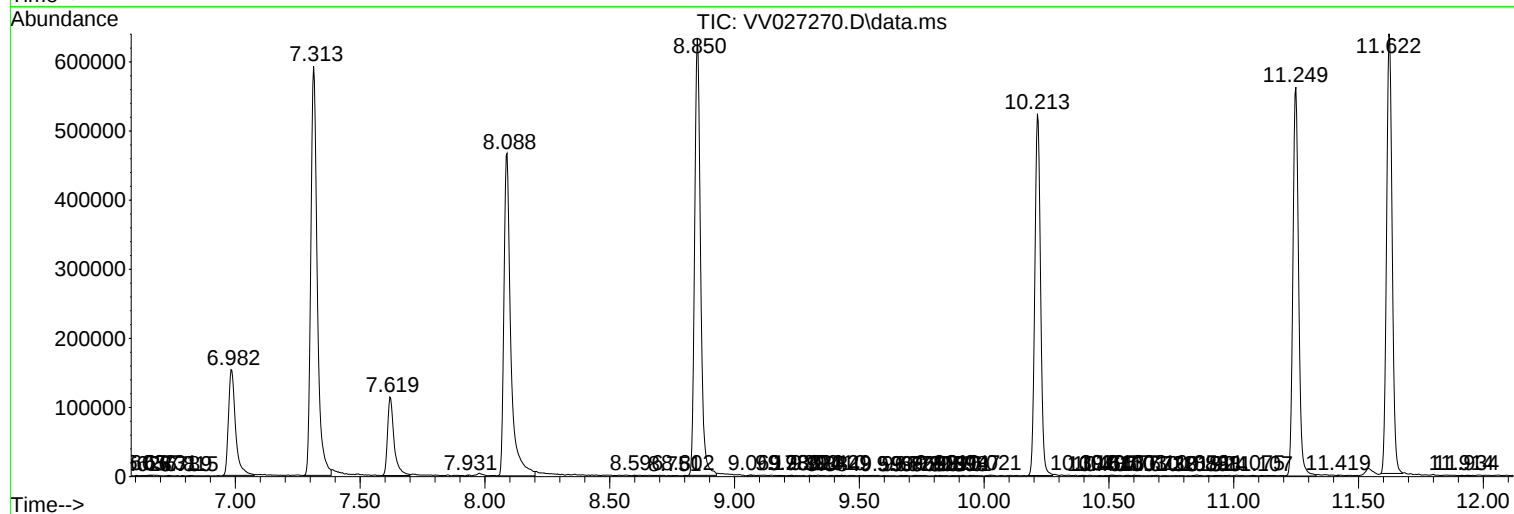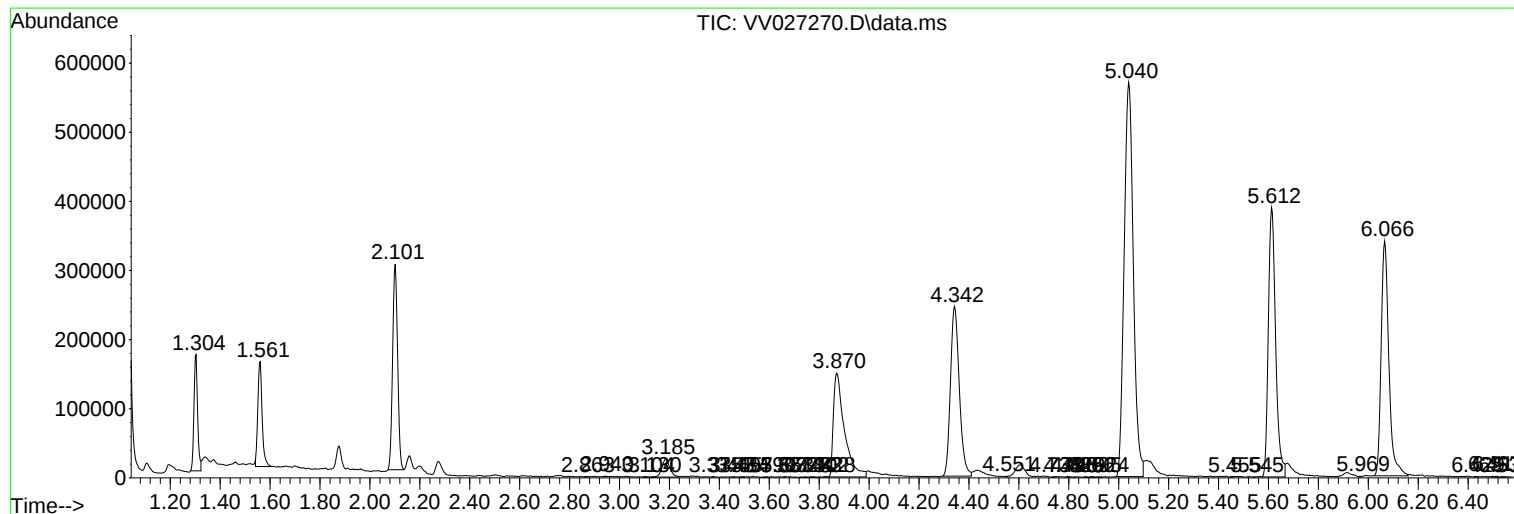

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081022\
Data File : VV027270.D
Acq On : 10 Aug 2022 20:25
Operator : SY/MD
Sample : N4144-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY147

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081022\
Data File : VV027270.D
Acq On : 10 Aug 2022 20:25
Operator : SY/MD
Sample : N4144-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY147

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------